

## Certificate of Analysis

### LudgerPure™ 2AA Labeled A2 Glycan


Cat. #: CAA-A2-01  
 Size: approx. 100 pmol

Batch: A887-01  
 Expiry Date: 06 JUL 2028


#### Alternative Names

A2G2S2, G2S2


#### Glycan Structure

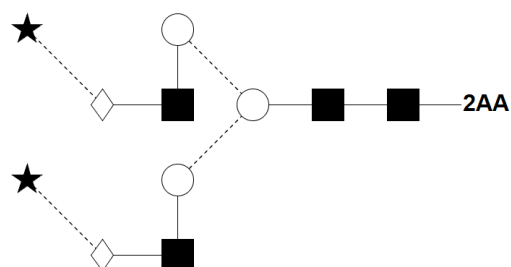

*Oxford Notation*

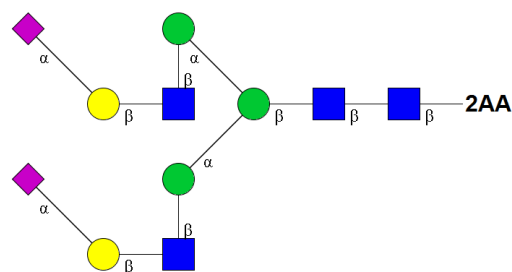


*CFG Notation*



*Text Notation*

**Purity:** 85.12% 2AA labeled A2 glycan, as assessed by HPLC - see Fig 1.

**Amount:** Sample vial determined to contain 91.9 pmols A2 glycan – Test performed 05 JUL 2023.

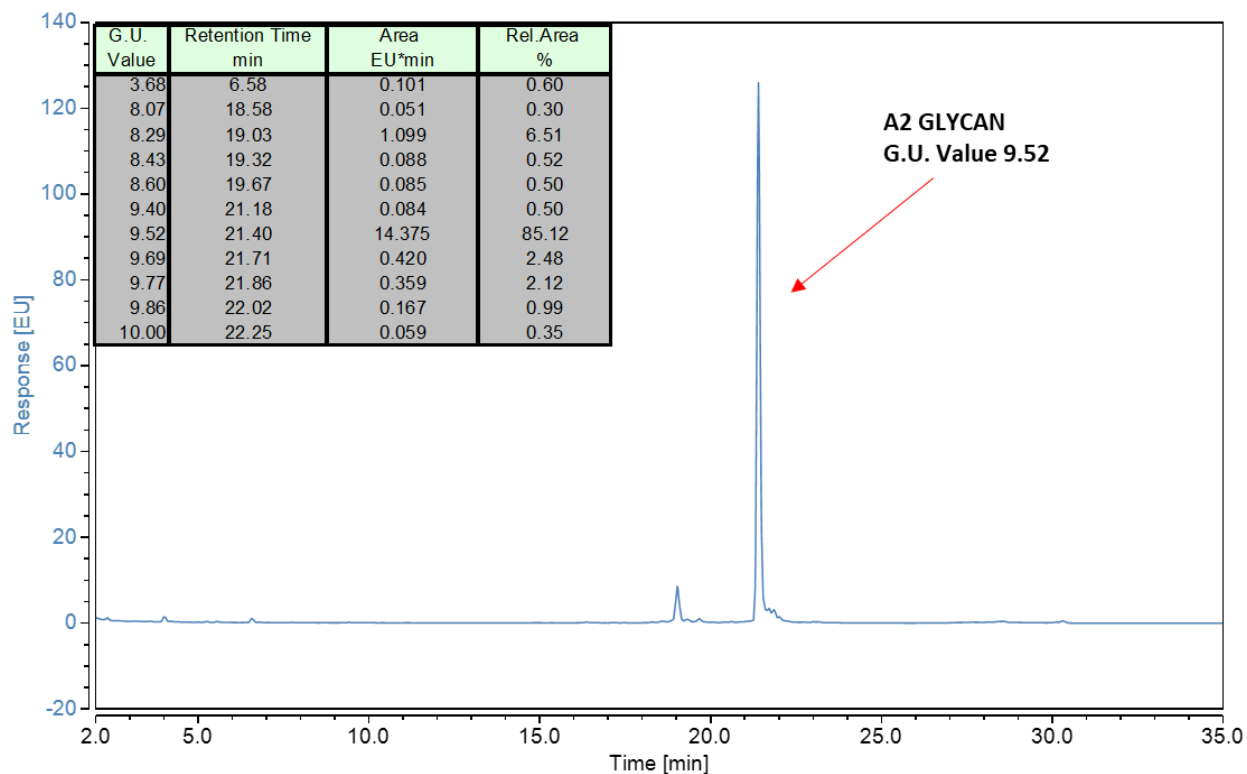

**Figure 1:** HILIC HPLC profile of 2AA labelled A2 glycan (see method conditions below) (Cat. #: CAA-A2-01, Batch A887-01).

\*A2 glycan structure identified by MALDI, MS & HPLC (GU value comparison to GlycoBase). This structure is drawn according to the scheme developed by Oxford-Dublin Glycobiology Laboratory (see Fig 2).

**2AA A2 peak seen above, eluted at 20.38 minutes, under the following conditions:**

**Column:** Waters BEH Glycan 1.7µm column (150mm)

**Flow:** 0.56mL/min.

**Temperature:** 60 °C

**Solvent A:** 50mM ammonium formate pH 4.4    **Solvent B:** 100 % acetonitrile

**Gradient:**

Time (min)	%B
0.0	78.0
1.5	78.0
24.8	58.0
25.8	40.0
25.9	78.0
31.0	78.0

**Detector:** Fluorescence

**Excitation wavelength:** 250 nm

**Emission wavelength:** 428 nm

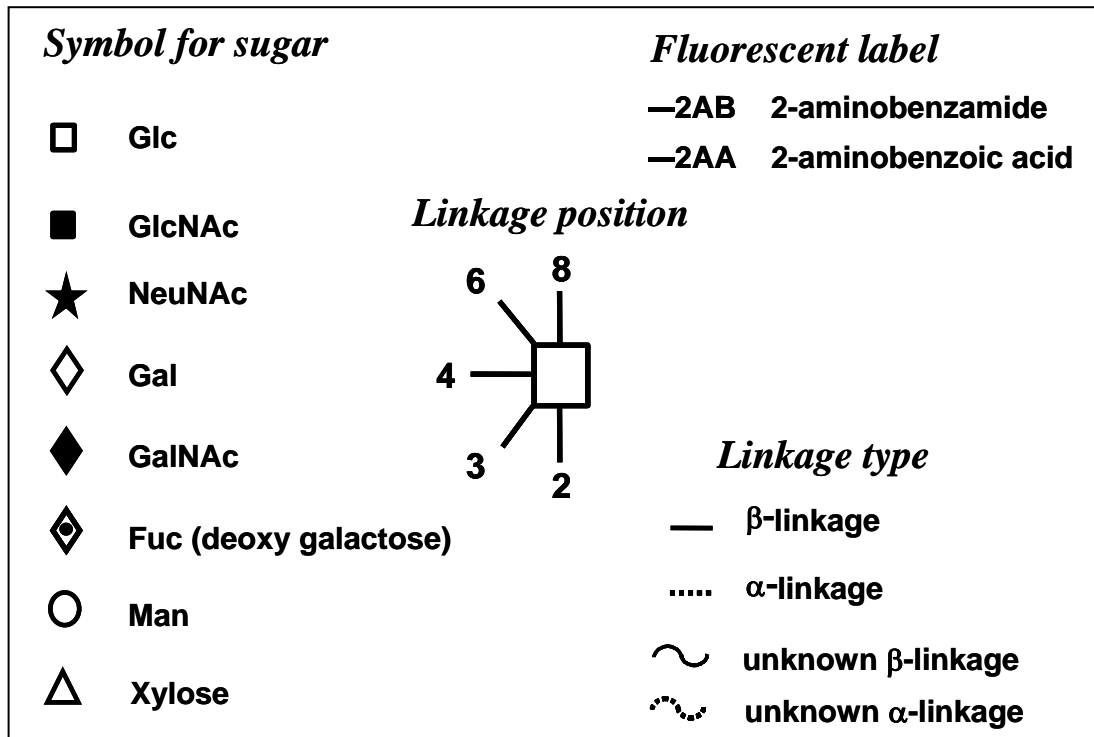


Figure 2: GlycoBase glycan structure key.