



Certificate of Analysis

LudgerSep N1 Amide HPLC Glycan Analysis Column

Cat. # : LS-N1-4.6x250

Serial # : A864-03

Size : 4.6 x 250mm

This column conforms to the specifications given in Ludger document # LS-N1-GUIDE.

Packed Solvent 75 % acetonitrile (aq)

Test Analysis

Flow Rate 1 ml / min

Eluent Isocratic 75 % acetonitrile (aq)

Pressure 5.9 MPa


Temperature 25 °C

Sample 1-Mannitol (at concentration of 2 g dm⁻³)

Sample Volume 20 µl

Detection Refractive Index

Inspection Chromatogram

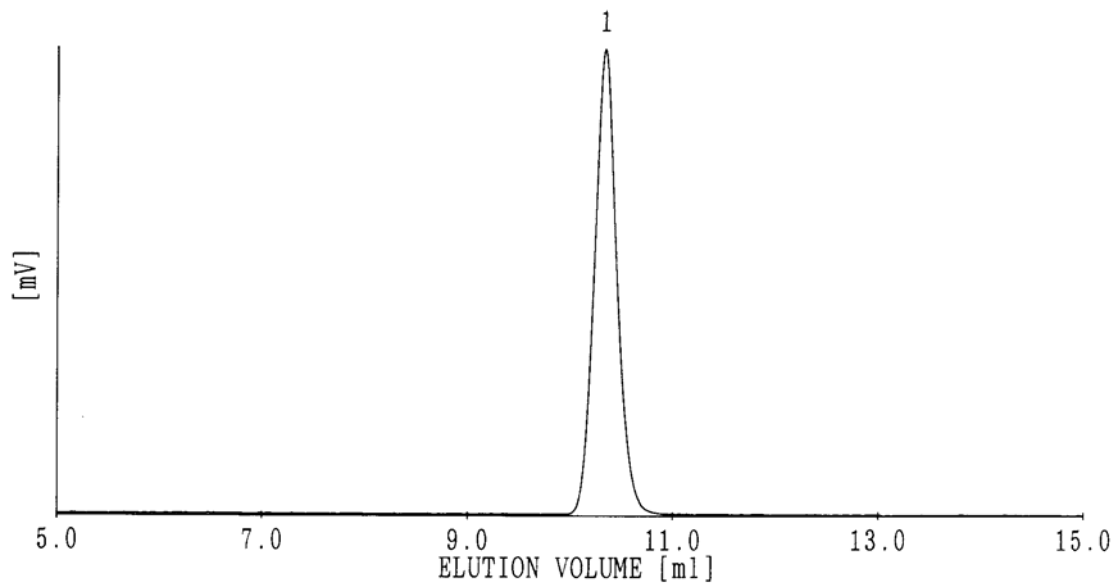

Theoretical Plates = 11343

Asymmetry Factor = 1.25