



## Certificate of Analysis

---

### LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. # : LS-N2-4.6x150

Serial # : B15R-13

Size : 4.6 x150mm

---

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

**Packed Solvent**      85 % acetonitrile (aq)

#### Test Analysis

**Flow Rate**            1.0 ml / min

**Eluent**                Isocratic 85 % acetonitrile (aq)

**Pressure**            4.9 MPa


**Temperature**        40 °C

**Sample**                Uracil 35mg/L

**Sample Volume**     10 µl

**Detection**            UV 254nm

#### Inspection Chromatogram

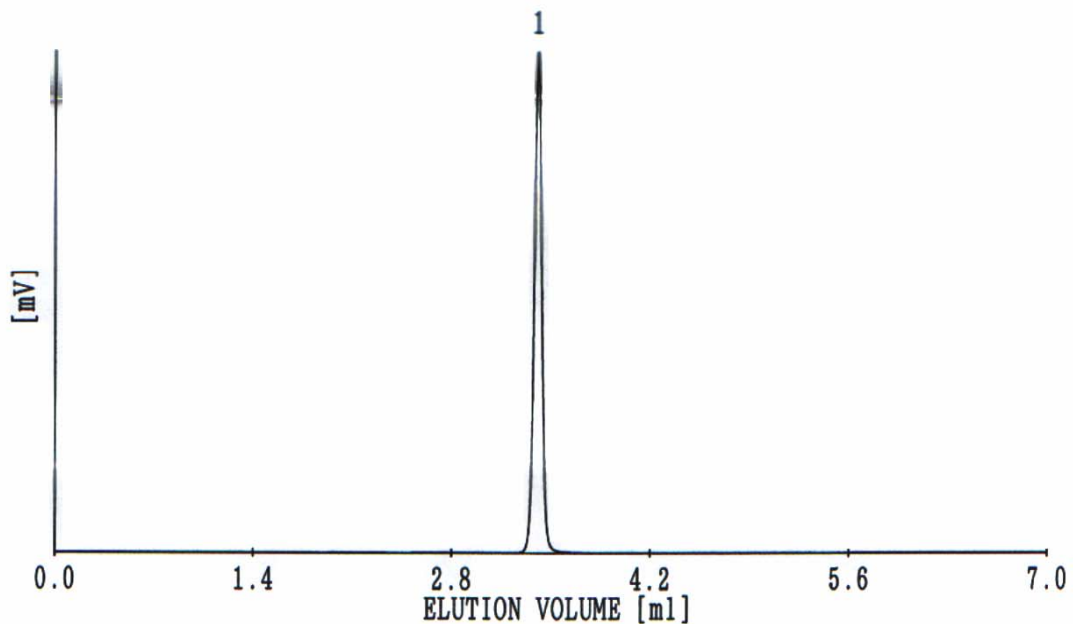

Theoretical Plates = 20437

Asymmetry Factor = 1.04