

Ludger

Certificate of Analysis

LudgerPure™ 2AB Labeled NGA2 Glycan



Cat. #: CAB-NGA2-01
Size: approx. 100 pmol

Batch: B4AU-02
Expiry: 30th Oct 2019

Alternative Names


A2

Structure

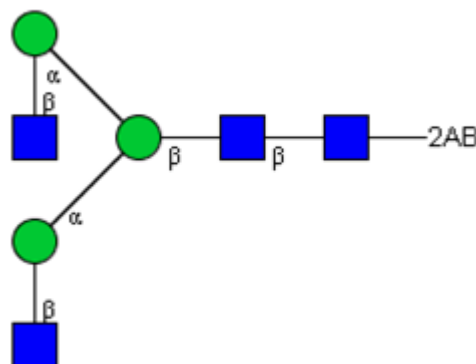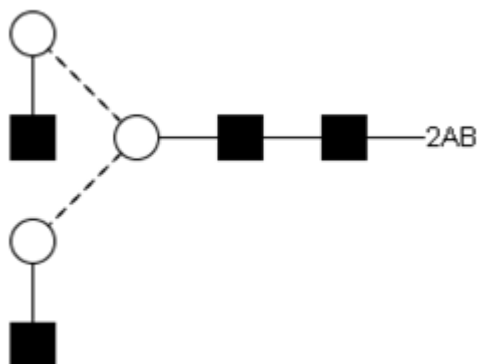

Oxford Notation

CFG Notation

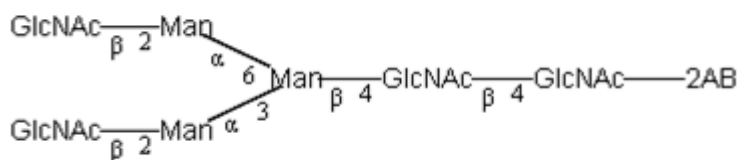

Text Notation

Purity: 91.84% 2AB labeled NGA2 glycan, as assessed by HPLC - see Fig 1.

Amount: Sample vial determined to contain 121.6 pmols NGA2 glycan – Test performed 6th November 2014

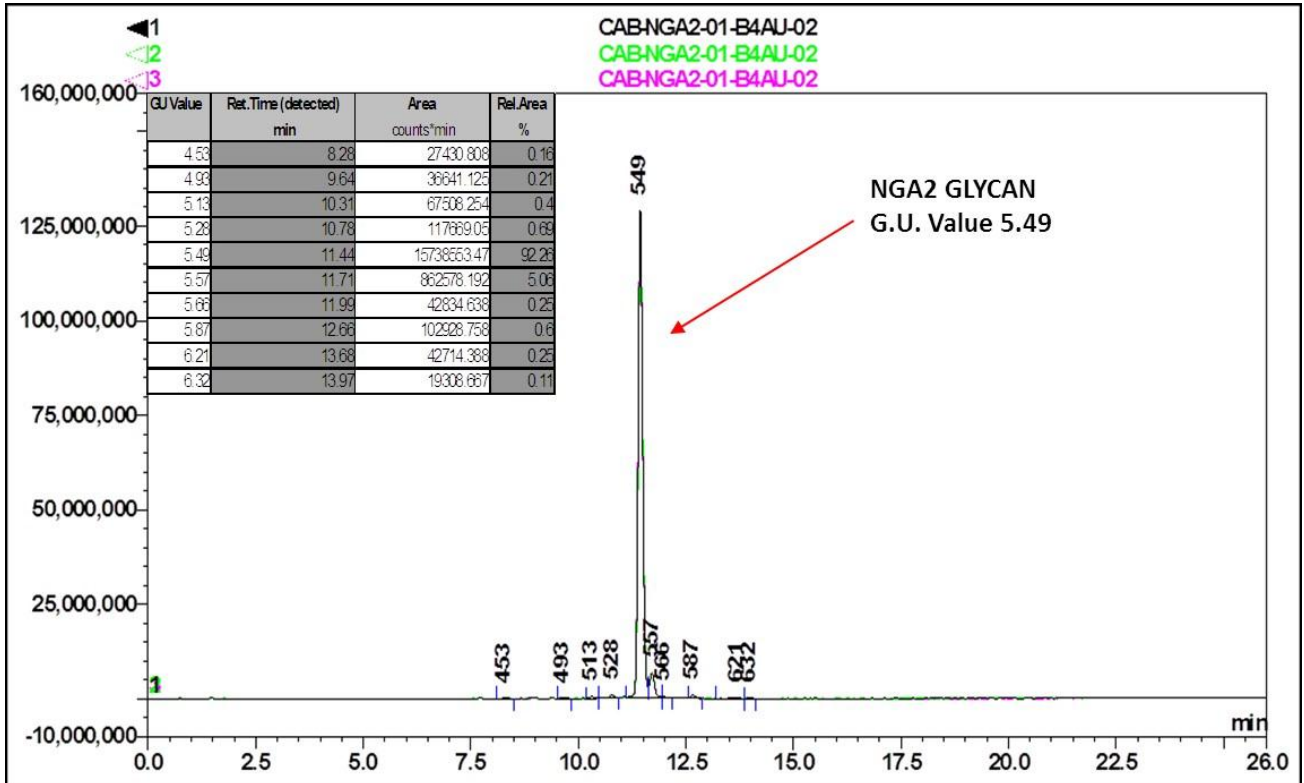


Figure 1: HILIC HPLC profile of 2AB labelled NGA2 glycan (see method conditions below) (Cat. #: CAB-NGA2-01, Batch B4AU-02).

*NGA2 glycan structure identified by MALDI, MS & HPLC (GU value comparison to GlycoBase). This structure is drawn according to the scheme developed by Oxford-Dublin Glycobiology Laboratory (see Fig 2).

2-AB NGA2 peak seen above, eluted at 11.44 minutes, under the following conditions:

Column: Waters BEH Glycan 1.7 μ m column (150mm) Flow:

0.56mL/min.

Temperature: 60 °C

Solvent A: 50mM ammonium formate pH 4.4

Solvent B: 100 % acetonitrile

Gradient:

Time (min)	%B
0.0	78.0
1.5	78.0
24.8	58.0
25.8	40.0
25.9	78.0
31.0	78.0

Detector: Dionex FLD-3000

Excitation wavelength: 250 nm

Emission wavelength: 428 nm

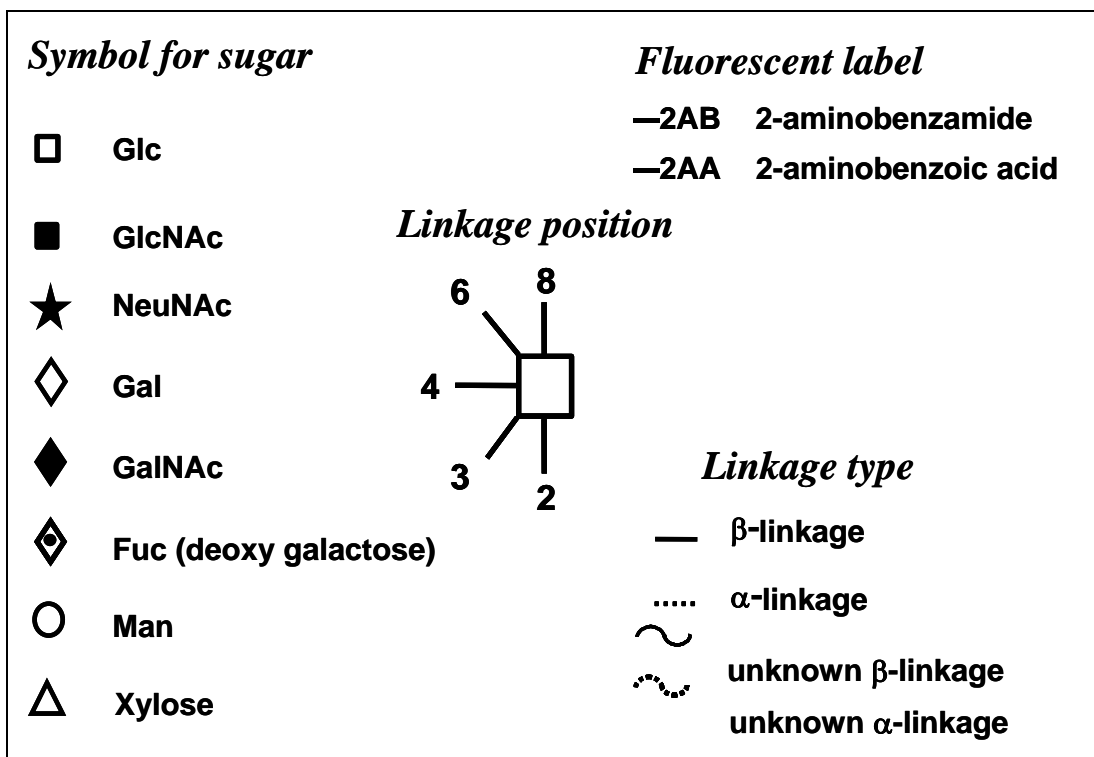


Figure 2: GlycoBase glycan structure key.