

Certificate of Analysis

LudgerPure™ 2AB Labeled NGA2F Glycan

Cat. #: CAB-NGA2F-01

Batch: B993-02


Size: approx. 100 pmol

Expiry Date: 03 Sep 2024


Alternative Names

FA2, G0F


Glycan Structure

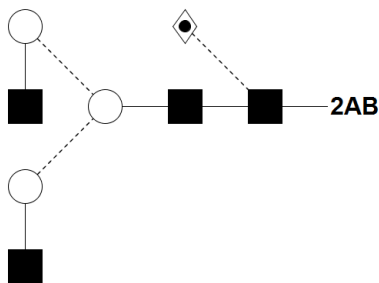

Oxford Notation

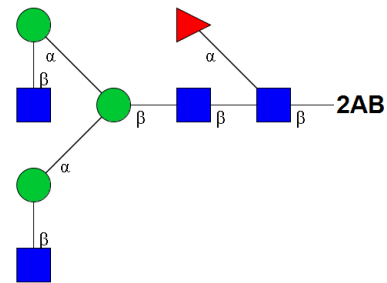

CFG Notation

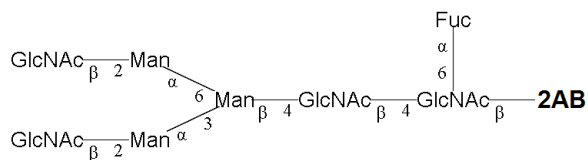

Text Notation

Purity: 98.3% 2AB labeled NGA2F glycan, as assessed by HPLC - see Fig 1.

Amount: Sample vial determined to contain 97.2pmols NGA2F glycan – Test performed 12 Sep 2019.

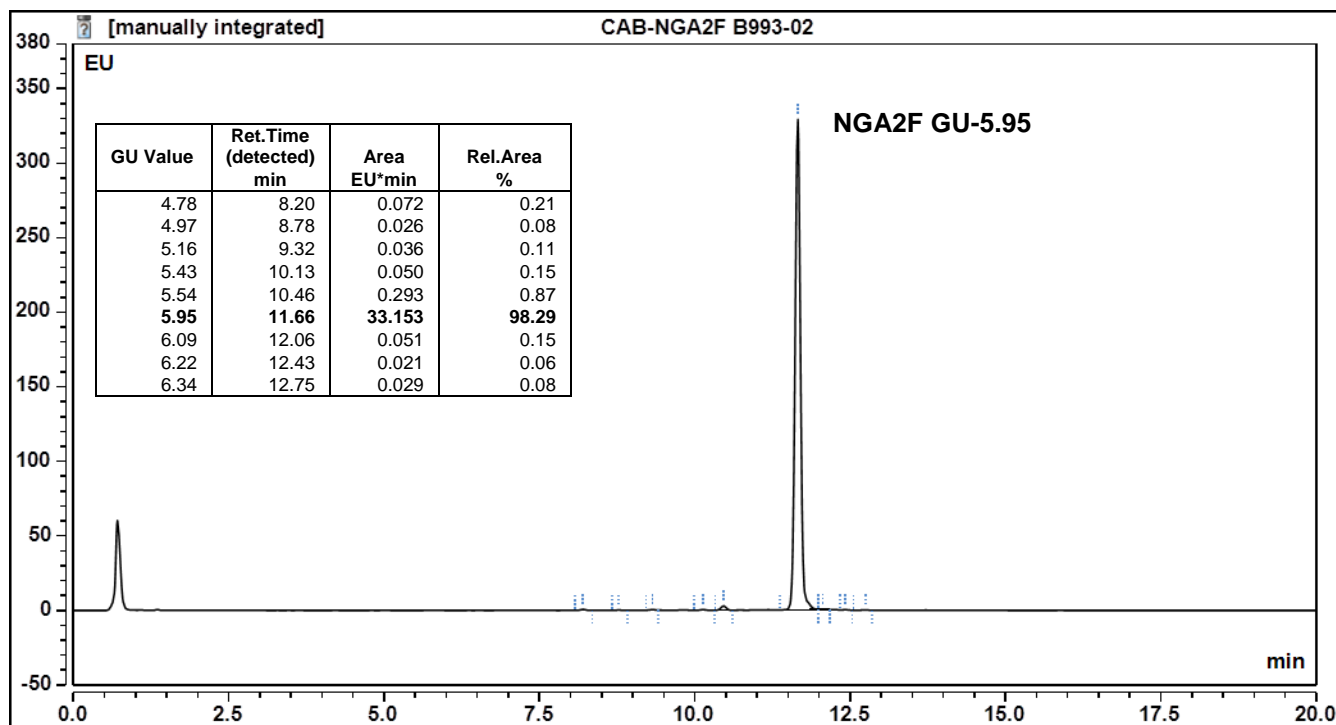


Figure 1: HILIC HPLC profile of 2AB labelled NGA2F glycan (see method conditions below) (Cat. #: CAB-NGA2F-01, Batch B993-02).

*NGA2F glycan structure identified by MALDI, MS & HPLC (GU value comparison to GlycoBase). This structure is drawn according to the scheme developed by Oxford-Dublin Glycobiology Laboratory (see Fig 2).

2-AB NGA2F peak seen above, eluted at 11.66 minutes, under the following conditions:

Column: Waters BEH Glycan 1.7µm column (150mm)

Flow: 0.56mL/min.

Temperature: 60 °C

Solvent A: 50mM ammonium formate pH 4.4 **Solvent B:** 100 % acetonitrile

Gradient:

Time (min)	%B
0.0	78.0
1.5	78.0
24.8	58.0
25.8	40.0
25.9	78.0
31.0	78.0

Detector: Fluorescence

Excitation wavelength: 250 nm

Emission wavelength: 428 nm

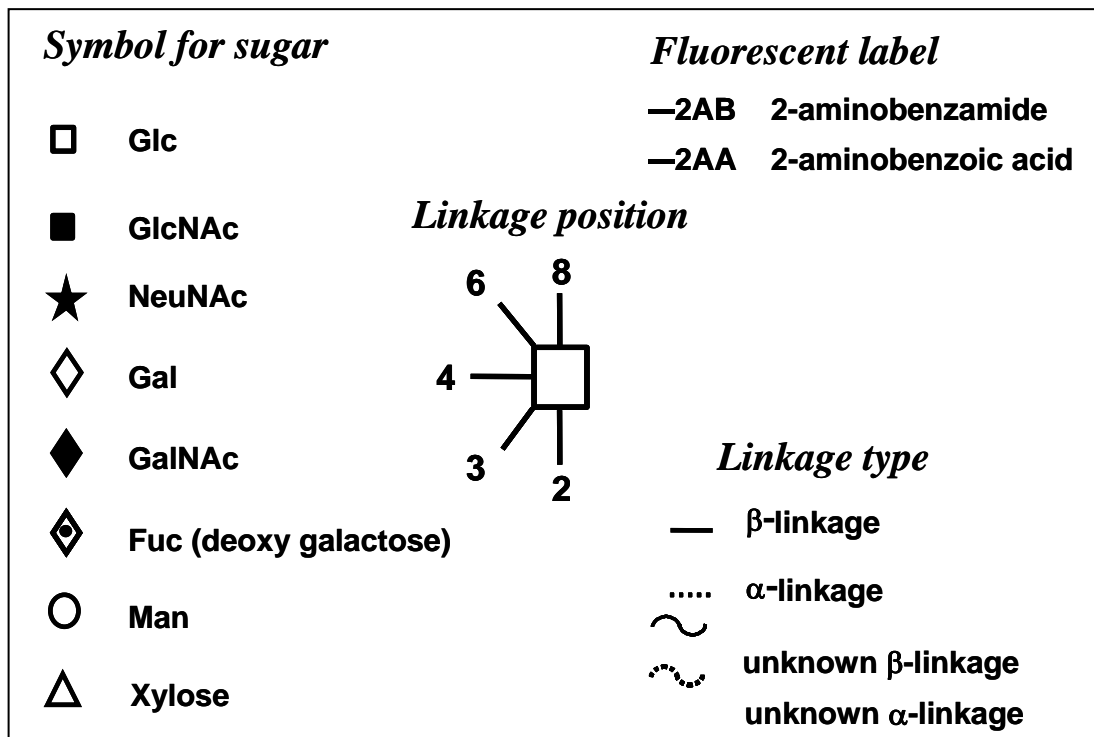


Figure 2: GlycoBase glycan structure key.