

Certificate of Analysis

NeuAc Standard

Cat. #: CM-NEUAC-01

Batch: B836-01

Size: 1.07 ± 0.09 nmol

Expiry Date: 06 Mar 2023

The N-acetylneuraminic acid standard is a quantitative standard of NIST-F and USP traceable Neu5Ac monosaccharide.

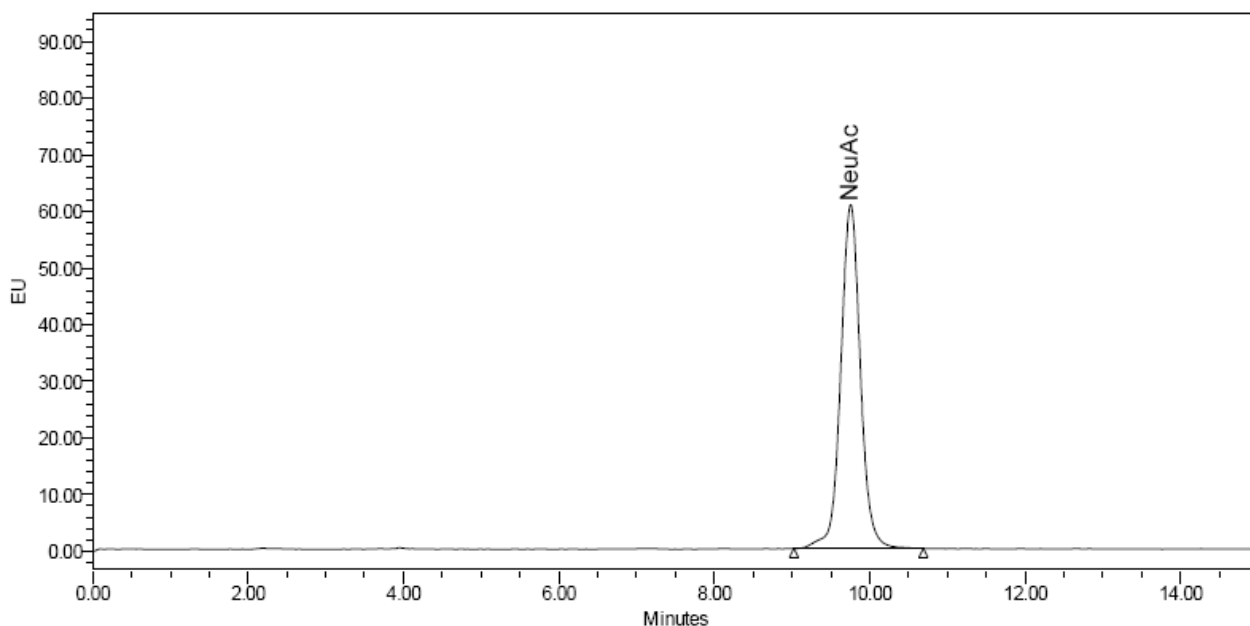


Figure 1: LudgerSep-R1 HPLC profile of 1,2-diamino-4,5-methylenedioxybenzene.2HCl (DMB) labeled NeuAc standard (Cat. #: CM-NEUAC-01, Batch B836-01).

Accuracy: This analysis was performed on 12 vials of CM-NEUAC-01.

The dispensed amount was determined as 1.07 ± 0.09 nmol NeuAc per vial.

Values are in nmols \pm standard deviation.

DMB labeled sialic acid standards eluted under the following HPLC conditions:**Column: LudgerSep R1 (Cat. #: LS-R1-4.6x150)**Flow: 0.5 ml/min.Temperature: 30 °CSolvent A: methanol:acetonitrile:water (7:9:84)Solvent B: acetonitrileGradient:

Time (min)	%B
0.0	0.0
19.0	0.0
19.5	90.0
23.5	90.0
24.0	0.0
30.0	0.0
35.0	0.0

Detector: FluorescenceExcitation wavelength: 373 nmEmission wavelength: 448 nm