

## Certificate of Analysis


### Sialic Acid Reference Panel

Cat. #: CM-SRP-01

Batch: B71N-07

Size: approx. 1.25 nmols

The sialic acid reference panel is a mixture of different sialic acids forms (as detailed on chromatogram below) sourced from bovine submaxillary mucin.

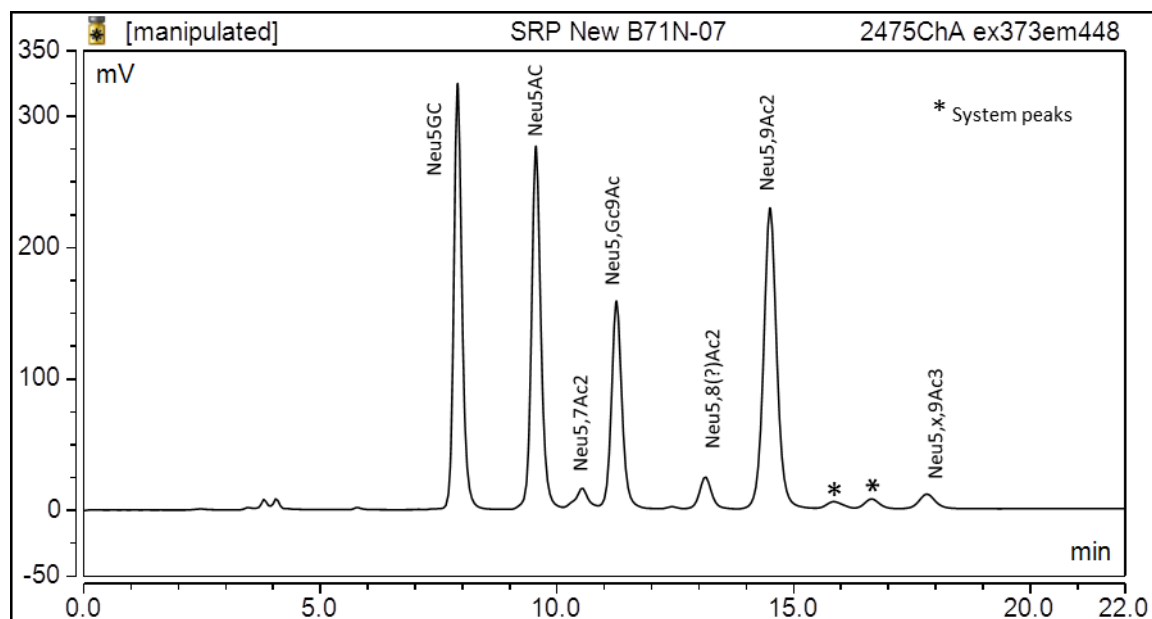

**Figure 1:** LudgerSep R1 HPLC profile of DMB labeled Sialic acid Reference Panel (Cat. #: CM-SRP-01, Batch B71N-07).

***DMB labeled SRP peaks seen above eluted under the following HPLC conditions:***

Column: LudgerSep R1 (LS-R1-4.6X150, B43I-04)

Flow: 0.5 ml/min.

Temperature: 30 °C

Solvent: Methanol:Acetonitrile:Water (7:9:84 v/v)

Fluorescence detector: Waters 2475 Excitation wavelength: 373 nm Emission wavelength: 448 nm