



# Ludger

## Certificate of Analysis

---

### LudgerSep C3 Anion Exchange HPLC Glycan Analysis Column

Cat. # : LS-C3-7.5x75

Batch # : B67P-01

Size : 7.5 x 75 mm

---

This column conforms to the specifications given in Ludger document # LS-C3-GUIDE.

**Packed Solvent**      Distilled water

#### Test Analysis

**Flow Rate**            1.0 ml / min

**Eluent**                35mmol/L NaCl+20mmol/ L Tris-HCl (pH 8.0)

**Pressure**             0.3 MPa


**Temperature**        25 °C

**Sample**                0.1 g/L Cytidine-5'- Monophosphate

**Sample Volume**     20 µl

**Detection**            UV at 254 nm

#### Inspection Chromatogram

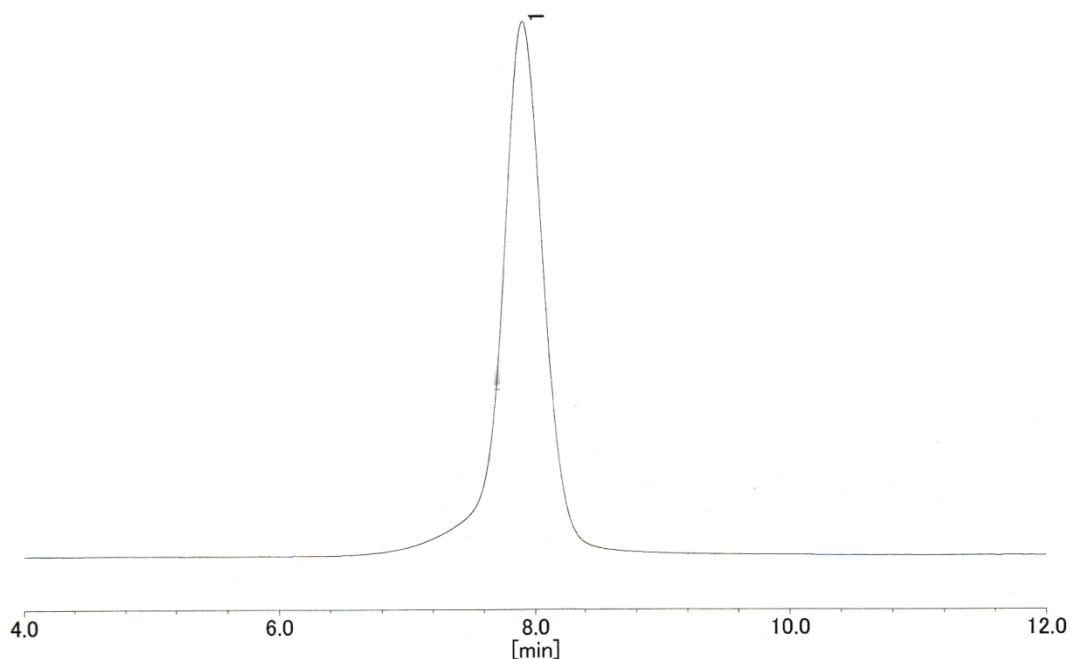

Theoretical Plates = 3,036

Asymmetry Factor = 0.96