

Certificate of Analysis**LudgerSep™ C3 Anion Exchange HPLC Glycan Analysis Column**

Cat. #: LS-C3-7.5x75

Batch: B95L-01

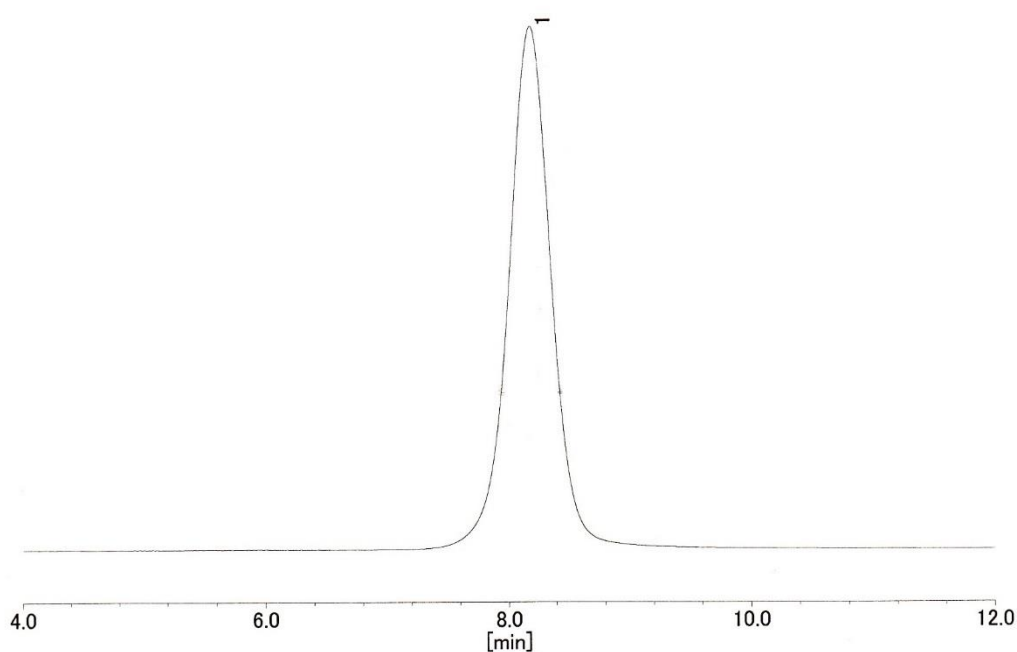
Size: 7.5 x 75 mm

This column conforms to the specifications given in Ludger document # LS-C3-GUIDE.

Packed Solvent Distilled water

Test Analysis

Flow Rate 1.0 ml / min
Eluent 35mmol/L NaCl+20mmol/ L Tris-HCl (pH 8.0)
Pressure 0.4 MPa
Temperature 25 °C
Sample 0.1 g/L Cytidine-5'- Monophosphate
Sample Volume 20 µl
Detection UV at 254 nm

Inspection Chromatogram

Theoretical Plates = 2809

Asymmetry Factor = 1.00