

Certificate of Analysis

LudgerSep[™] C3 Anion Exchange HPLC Glycan Analysis Column

Cat. #: LS-C3-7.5x75

Batch: B98N-01


Size: 7.5 x 75 mm

This column conforms to the specifications given in Ludger document # LS-C3-GUIDE.

Packed Solvent Distilled water

Test Analysis

Flow Rate	1.0 ml / min
Eluent	35mmol/L NaCl+20mmol/ L Tris-HCl (pH 8.0)
Pressure	0.3 MPa
Temperature	25 °C
Sample	0.1 g/L Cytidine-5'- Monophosphate
Sample Volume	20 µl
Detection	UV at 254 nm

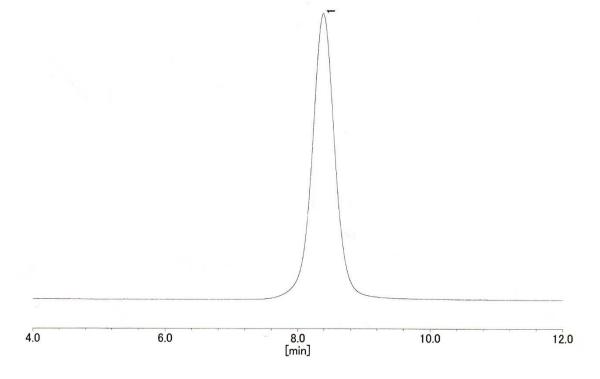

Theoretical Plates = 3050