



Ludger

Certificate of Analysis

LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. #: LS-N2-2.0x150

Serial #: B24R-01

Size: 2.0 x150mm

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

Packed Solvent 85 % acetonitrile (aq)

Test Analysis

Flow Rate 0.2 ml / min

Eluent Isocratic 85 % acetonitrile (aq)

Pressure 4.9 MPa


Temperature 25 °C

Sample Uracil 35mg/L

Sample Volume 2 µl

Detection UV 254nm

Inspection Chromatogram

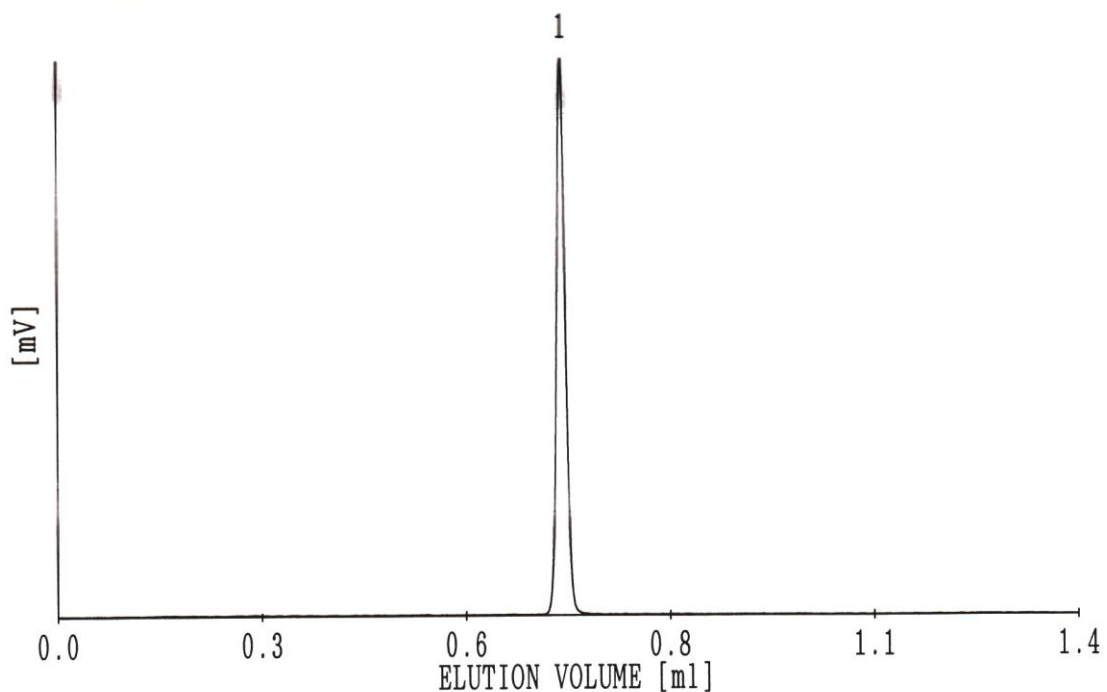

Theoretical Plates = 15797

Asymmetry Factor = 1.09