



Ludger

## Certificate of Analysis

---

### LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. #: LS-N2-2.0x150

Serial #: B24R-03

Size: 2.0 x150mm

---

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

**Packed Solvent** 85 % acetonitrile (aq)

#### Test Analysis

**Flow Rate** 0.2 ml / min

**Eluent** Isocratic 85 % acetonitrile (aq)

**Pressure** 4.8 MPa


**Temperature** 25 °C

**Sample** Uracil 35mg/L

**Sample Volume** 2 µl

**Detection** UV 254nm

#### Inspection Chromatogram

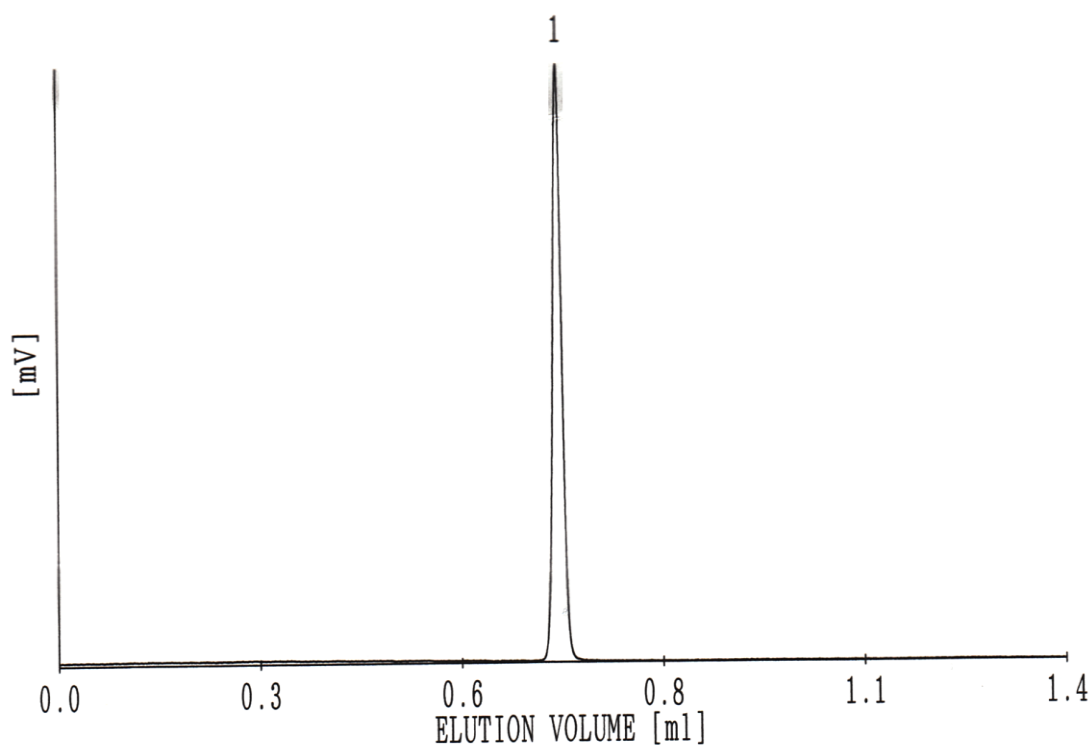

Theoretical Plates = 14795

Asymmetry Factor = 1.03