



Ludger

## Certificate of Analysis

---

### LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. #: LS-N2-2.0x150

Serial #: B24R-04

Size: 2.0 x150mm

---

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

**Packed Solvent**      85 % acetonitrile (aq)

#### Test Analysis

**Flow Rate**            0.2 ml / min

**Eluent**                Isocratic 85 % acetonitrile (aq)

**Pressure**            4.7 MPa


**Temperature**        25 °C

**Sample**                Uracil 35mg/L

**Sample Volume**     2 µl

**Detection**            UV 254nm

#### Inspection Chromatogram

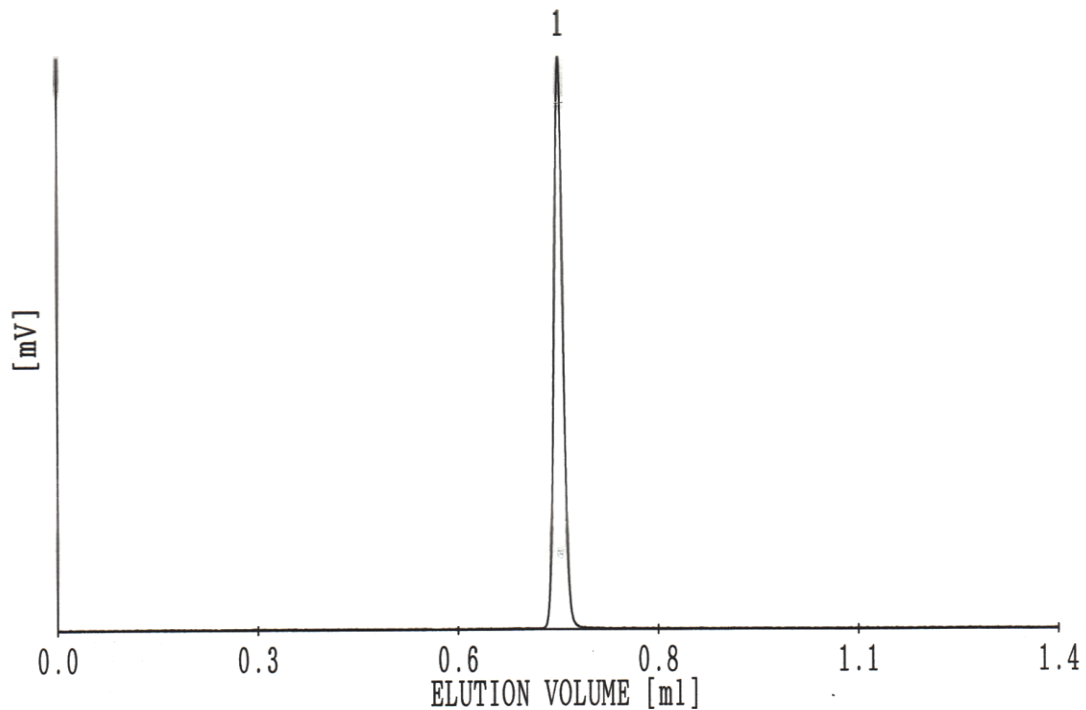

Theoretical Plates = 15364

Asymmetry Factor = 1.17