



## Certificate of Analysis

---

### LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. #: LS-N2-4.6x150

Serial #: B556-06

Size: 4.6 x150mm

---

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

**Packed Solvent** 85 % acetonitrile (aq)

#### Test Analysis

**Flow Rate** 1.0 ml / min

**Eluent** Isocratic 85 % acetonitrile (aq)

**Pressure** 4.7 MPa


**Temperature** 40 °C

**Sample** Uracil 35mg/L

**Sample Volume** 10  $\mu$ l

**Detection** UV 254nm

#### Inspection Chromatogram

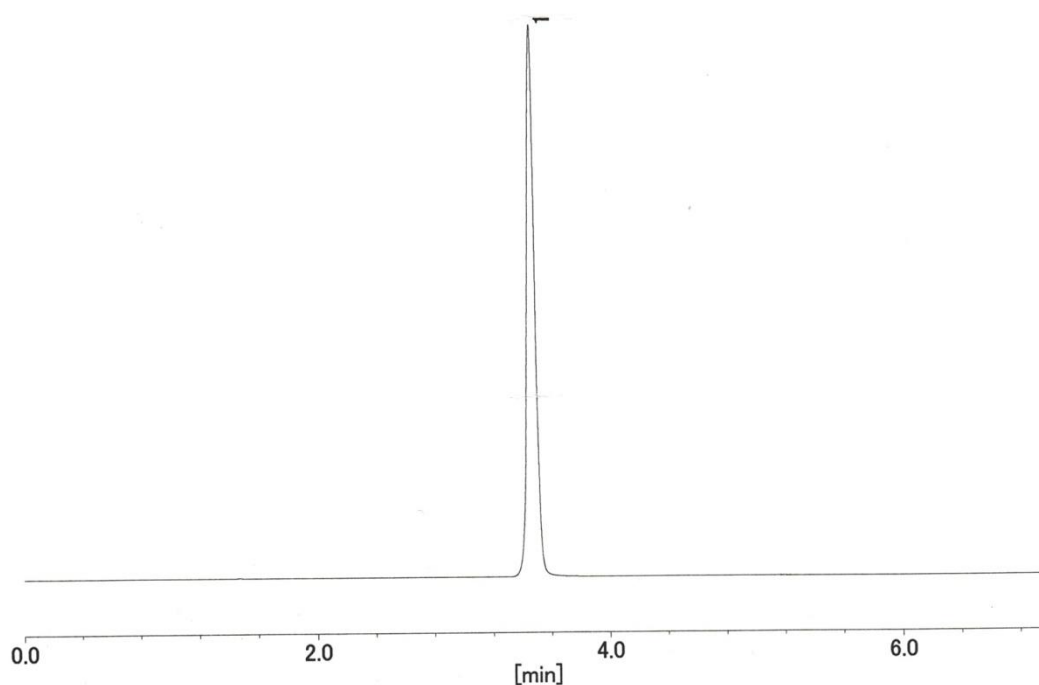

Theoretical Plates = 20066

Asymmetry Factor = 0.91