



## Certificate of Analysis

---

# LudgerSep N2 Amide HPLC Glycan Analysis Column

Cat. #: LS-N2-4.6x150

Serial #: B92E-09

Size: 4.6 x150mm

---

This column conforms to the specifications given in Ludger document # LS-N2-GUIDE.

**Packed Solvent**      85 % acetonitrile (aq)

### Test Analysis

**Flow Rate**            1.0 ml / min

**Eluent**                Isocratic 85 % acetonitrile (aq)

**Pressure**             5.0 MPa


**Temperature**        40 °C

**Sample**                Uracil 35mg/L

**Sample Volume**     10  $\mu$ l

**Detection**            UV 254nm

### Inspection Chromatogram

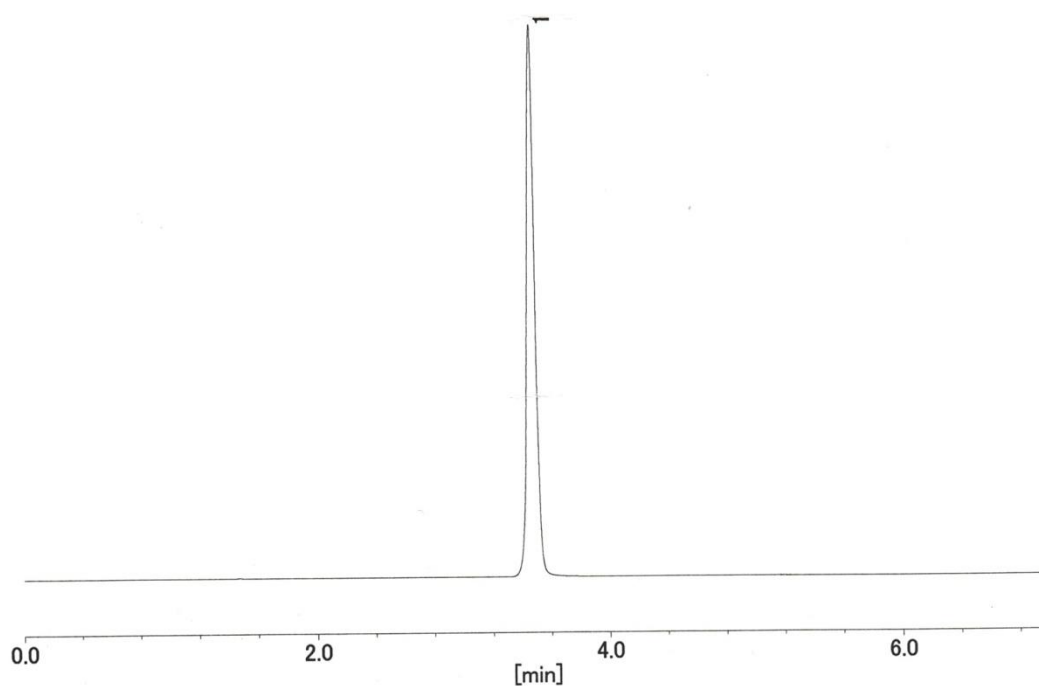

Theoretical Plates = 20002

Asymmetry Factor = 1.08