



Certificate of Analysis

LudgerSep R1 HPLC Column for Glycan Analysis

Cat. # : LS-R1-4.6x150

Batch # : B49T-01

Size : 4.6 x 150 mm

This column conforms to the specifications given in Ludger document # LS-R1-GUIDE.

Packed Solvent 60 % acetonitrile (aq)

Test Analysis

Flow Rate 1.25 ml / min


Eluent Isocratic 60 % acetonitrile (aq)

Pressure 2440 psi

Temperature Ambient

Sample Volume 5 μ l

Detection UV at 254nm

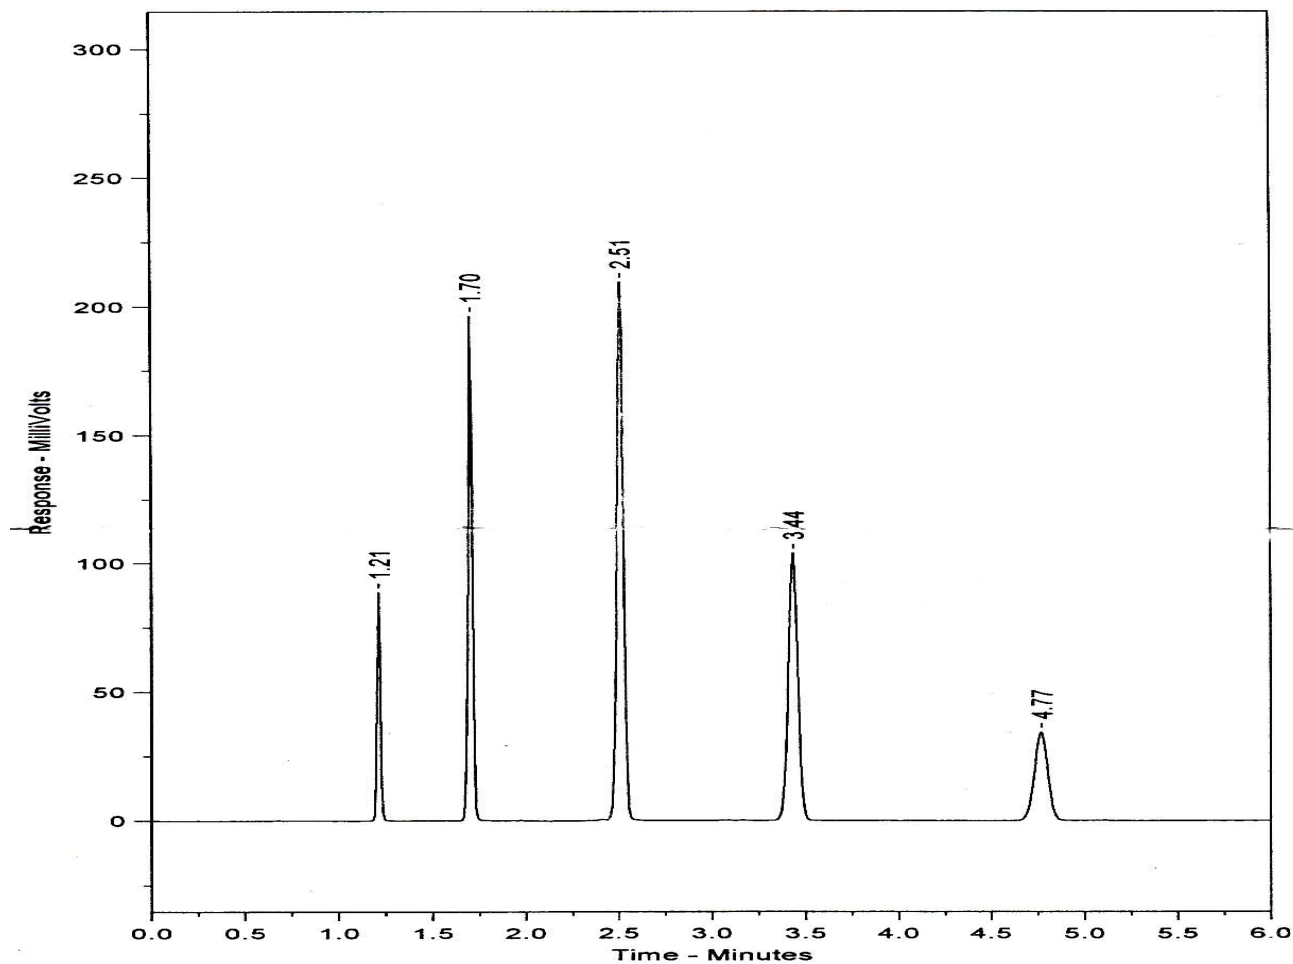

Peak No	Peak Name	Retention time (minutes)	Capacity Factor
1	Theophyline	1.21	0.00
2	p-Nitroaniline	1.70	0.40
3	Methyl Benzoate	2.51	1.07
4	Phenetole	3.44	1.83
5	o-Xylene	4.77	2.93

Efficiency o-Xylene (n/m) = 137468

Asymmetry Factor (10%) o-Xylene = 0.952