



Certificate of Analysis

LudgerSep™ R1 HPLC Column for Glycan Analysis

Cat. #: LS-R1-4.6x150

Batch: B85L-03

Size: 4.6 x 150 mm

This column conforms to the specifications given in Ludger document # LS-R1-GUIDE.

Packed Solvent 60 % acetonitrile (aq)

Test Analysis

Flow Rate 1.25 ml / min


Eluent Isocratic 60 % acetonitrile (aq)

Pressure 2653 psi

Temperature Ambient

Sample Volume 5 µl

Detection UV at 254nm

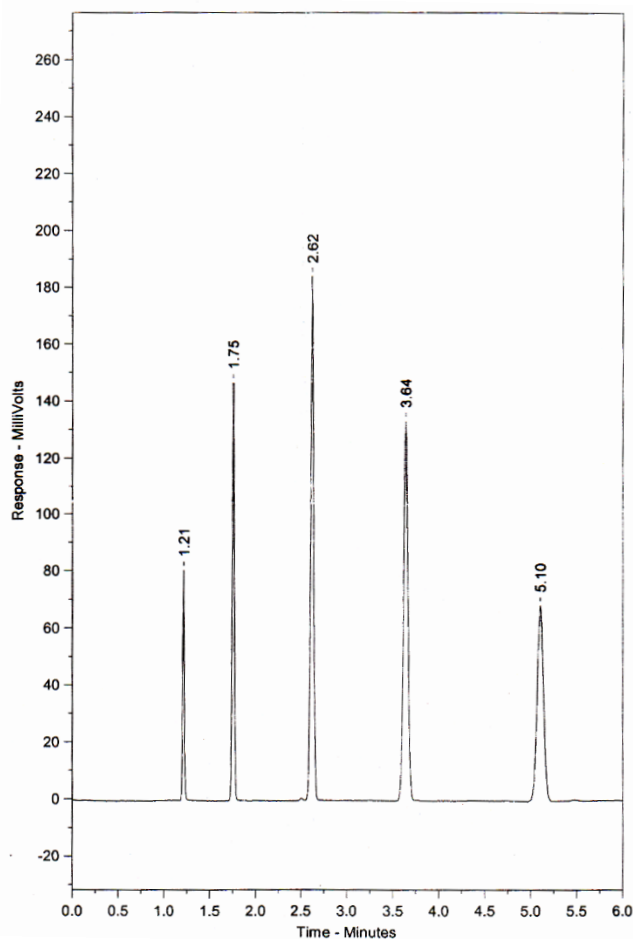

Peak No	Peak Name	Retention time (minutes)	Capacity Factor
1	Theophylline	1.21	0.00
2	p-Nitroaniline	1.75	0.45
3	Methyl Benzoate	2.62	1.16
4	Phenetole	3.64	2.00
5	o-Xylene	5.10	3.21

Efficiency o-Xylene (n/m) = 157728

Asymmetry Factor (10%) o-Xylene = 1.028