



Certificate of Analysis

LudgerSep™ R1 HPLC Column for Glycan Analysis

Cat. #: LS-R1-4.6x150

Batch: B88N-03

Size: 4.6 x 150 mm

This column conforms to the specifications given in Ludger document # LS-R1-GUIDE.

Packed Solvent 60 % acetonitrile (aq)

Test Analysis

Flow Rate 1.25 ml / min


Eluent Isocratic 60 % acetonitrile (aq)

Pressure 2538 psi

Temperature Ambient

Sample Volume 5 µl

Detection UV at 254nm

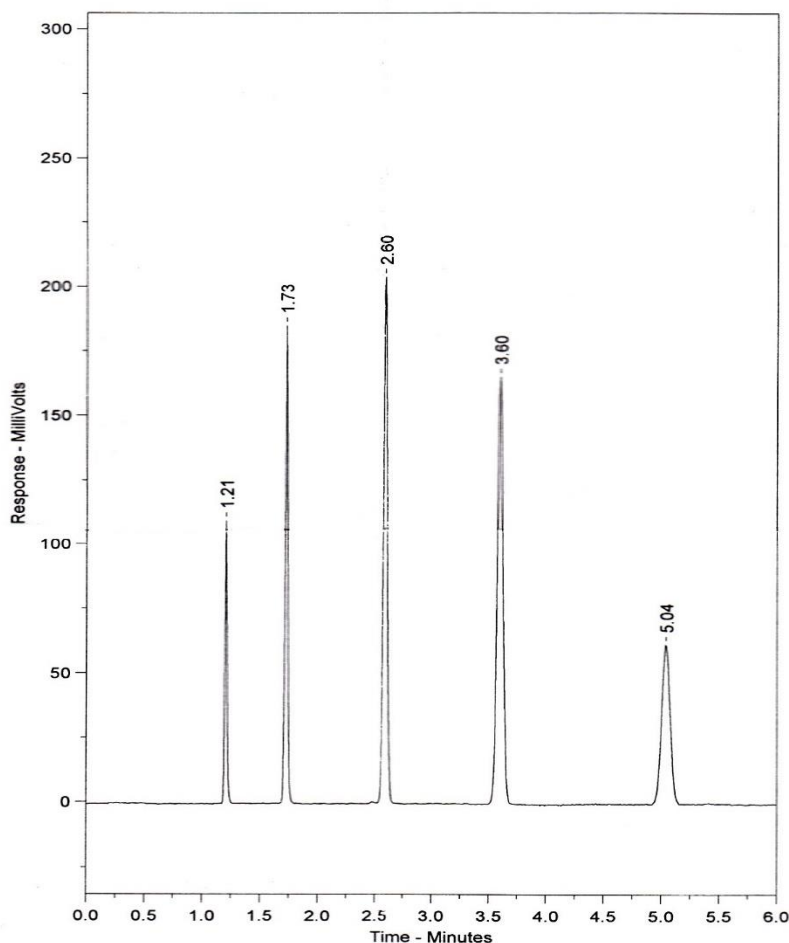

Peak No	Peak Name	Retention time (minutes)	Capacity Factor
1	Theophylline	1.21	0.00
2	p-Nitroaniline	1.73	0.43
3	Methyl Benzoate	2.60	1.15
4	Phenetole	3.60	1.99
5	o-Xylene	5.04	3.18

Efficiency o-Xylene (n/m) = 146548

Asymmetry Factor (10%) o-Xylene = 1.074