



## Certificate of Analysis

---

### LudgerSep R2 HPLC Column for Glycan Analysis

Cat. #: LS-R2-4.6x150

Batch #: B69K-07

Size: 4.6 x 150 mm

---

This column conforms to the specifications given in Ludger document # LS-R2-GUIDE.

**Packed Solvent** 60 % acetonitrile (aq)

#### Test Analysis

**Flow Rate** 1.25 ml / min


**Eluent** Isocratic 60 % acetonitrile (aq)

**Pressure** 1760 psi

**Temperature** Ambient

**Sample Volume** 2.5  $\mu$ l

**Detection** UV at 254nm

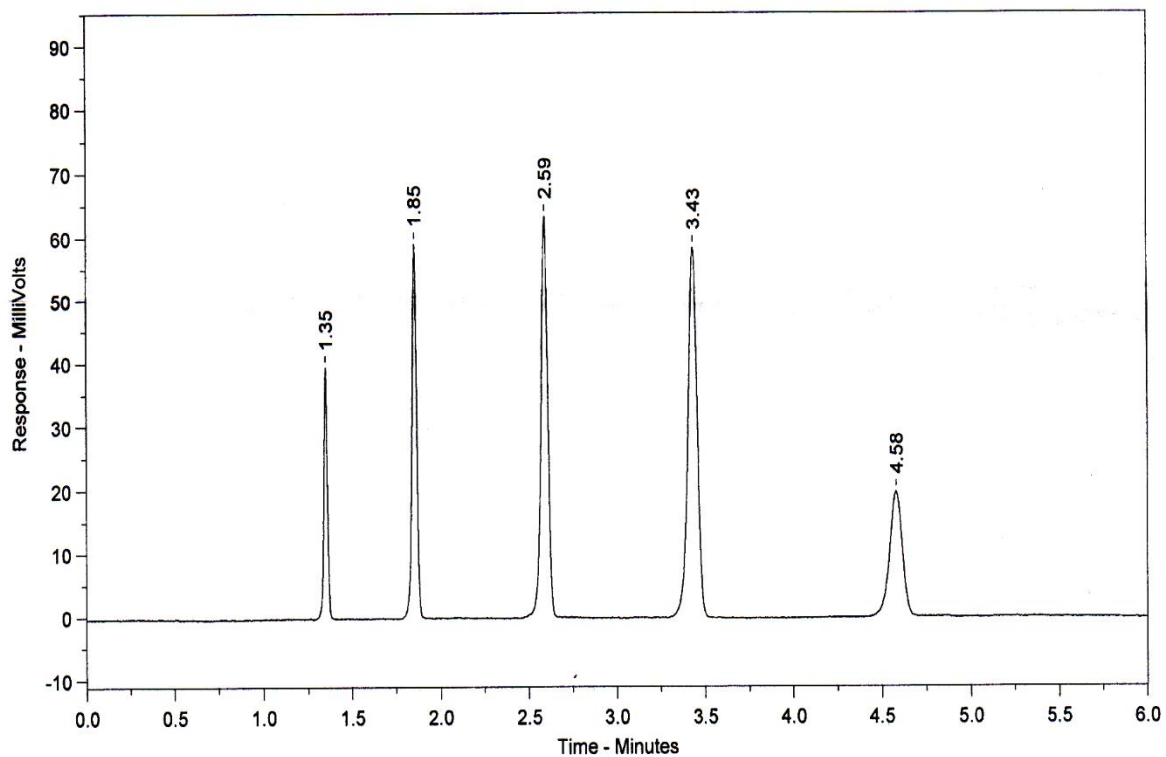

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	1.35	0.92
2	p-Nitroaniline	1.85	0.94
3	Methyl Benzoate	2.59	0.87
4	Phenetole	3.43	0.90
5	o-Xylene	4.58	0.91

Efficiency o-Xylene (n/m) = 132329

Asymmetry Factor (5%) o-Xylene = 0.91