



Certificate of Analysis

LudgerSep R2 HPLC Column for Glycan Analysis

Cat. #: LS-R2-4.6x150

Batch #: B79J-02

Size: 4.6 x 150 mm

This column conforms to the specifications given in Ludger document # LS-R2-GUIDE.

Packed Solvent 60 % acetonitrile (aq)

Test Analysis

Flow Rate 1.25 ml / min


Eluent Isocratic 60 % acetonitrile (aq)

Pressure 1780 psi

Temperature Ambient

Sample Volume 2.5 μ l

Detection UV at 254nm

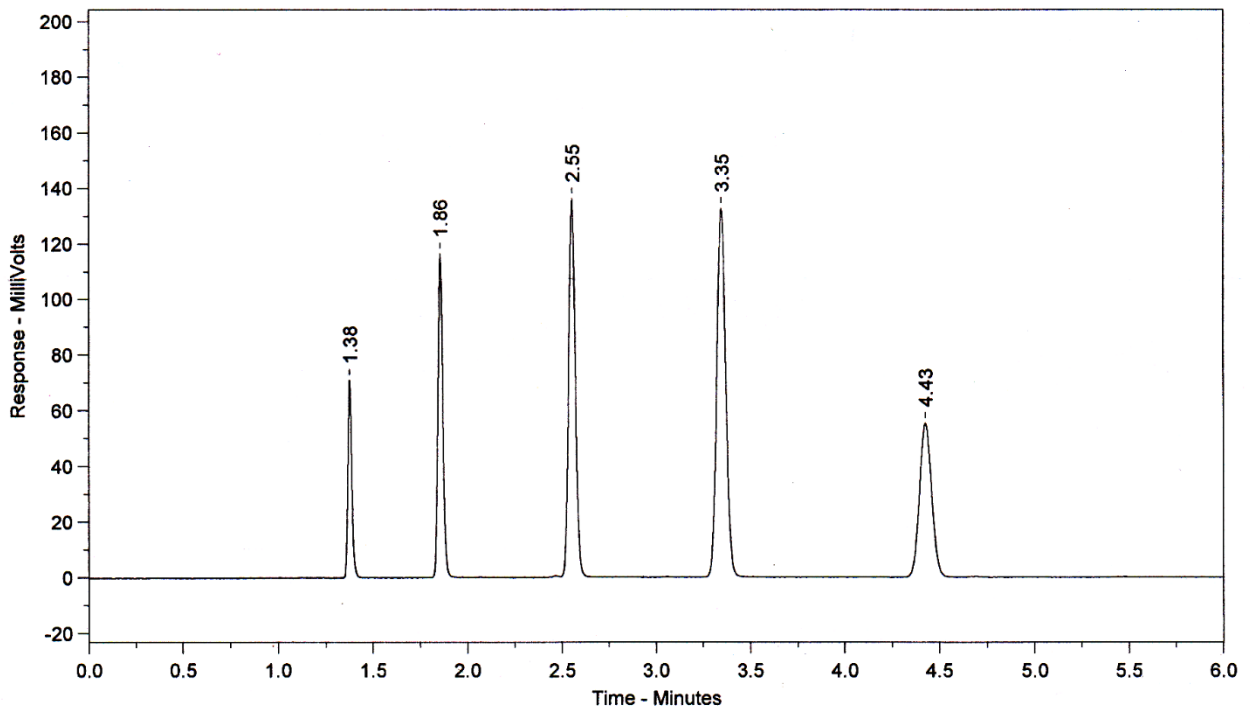

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophyline	1.38	1.32
2	p-Nitroaniline	1.86	1.12
3	Methyl Benzoate	2.55	1.09
4	Phenetole	3.35	1.07
5	o-Xylene	4.43	1.04

Efficiency o-Xylene (n/m) = 149632

Asymmetry Factor (5%) o-Xylene = 1.04