



Certificate of Analysis

LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x100

Batch #: B4AA-03

Size: 2.1 x 100 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

Packed Solvent 50 % acetonitrile (aq)

Test Analysis

Flow Rate 500ul / min


Eluent Isocratic 50 % acetonitrile (aq)

Pressure 7468 psi

Temperature Ambient

Sample Volume 1 μ l

Detection UV at 254nm

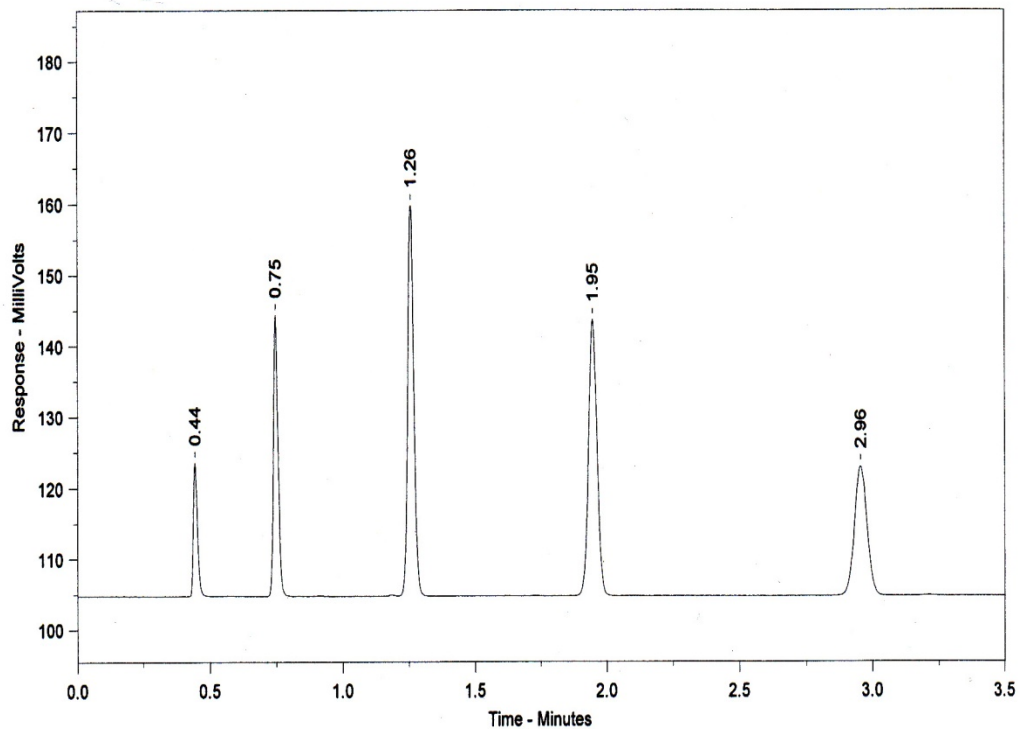

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophyline	0.44	1.33
2	p-Nitroaniline	0.75	1.20
3	Methyl Benzoate	1.26	1.07
4	Phenetole	1.95	1.03
5	o-Xylene	2.96	1.02

Efficiency o-Xylene (n/m) = 181948

Tailing Factor (5%) o-Xylene = 1.02