



Ludger

## Certificate of Analysis

---

### LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x100

Batch #: B51T-03

Size: 2.1 x 100 mm

---

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent** 50 % acetonitrile (aq)

#### Test Analysis

**Flow Rate** 500ul / min


**Eluent** Isocratic 50 % acetonitrile (aq)

**Pressure** 7864 psi

**Temperature** Ambient

**Sample Volume** 1  $\mu$ l

**Detection** UV at 254nm

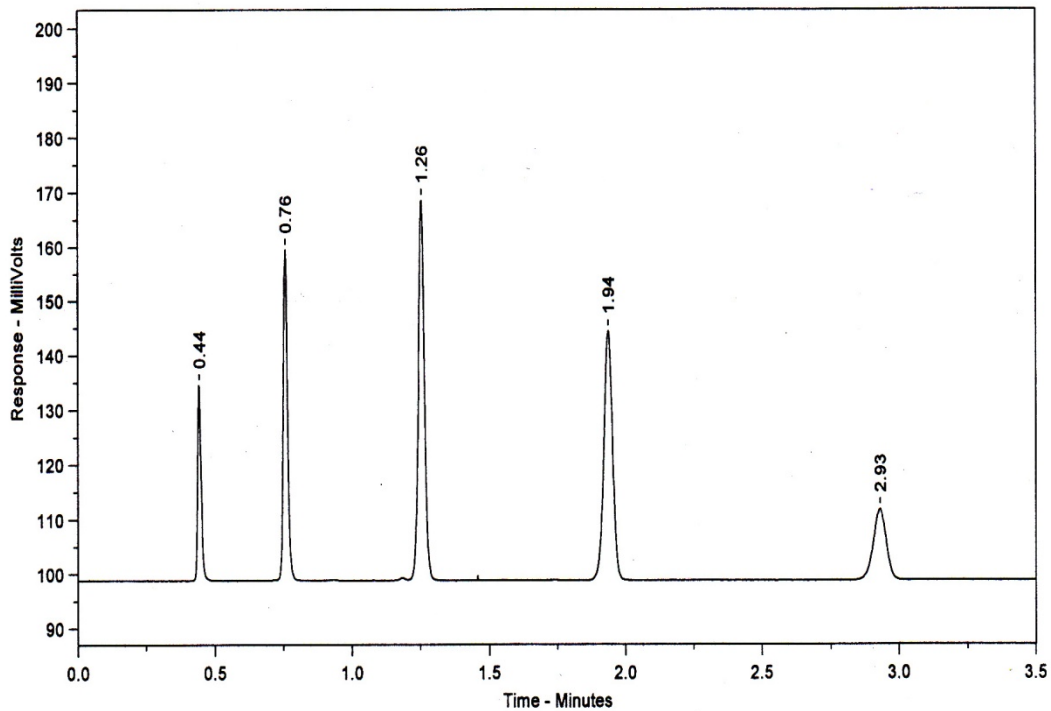

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophyline	0.44	1.35
2	p-Nitroaniline	0.76	1.10
3	Methyl Benzoate	1.26	1.01
4	Phenetole	1.94	0.96
5	o-Xylene	2.93	0.96

Efficiency o-Xylene (n/m) = 176942

Tailing Factor (5%) o-Xylene = 0.96