

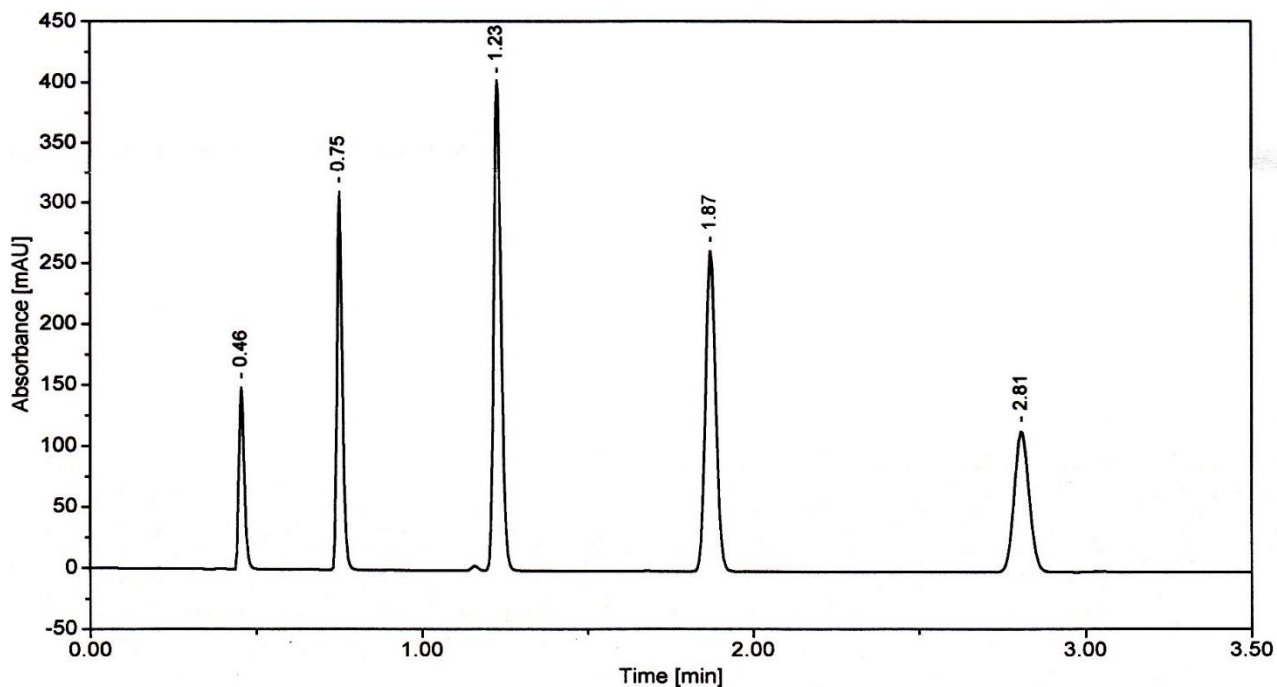
**Certificate of Analysis****LudgerSep™ UR2 UHPLC Column for Glycan Analysis**

Cat. #: LS-UR2-2.1x100

Batch: B87G-05

Size: 2.1 x 100 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent** 50 % acetonitrile (aq)**Test Analysis****Flow Rate** 500ul / min**Eluent** Isocratic 50 % acetonitrile (aq)**Pressure** 7436 psi**Sample Volume** 1 µl**Detection** UV at 254nm

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	0.46	1.25
2	p-Nitroaniline	0.75	1.24
3	Methyl Benzoate	1.23	1.16
4	Phenetole	1.87	1.07
5	o-Xylene	2.81	1.06

Efficiency o-Xylene (n/m) = 186140

Tailing Factor (5%) o-Xylene = 1.06