

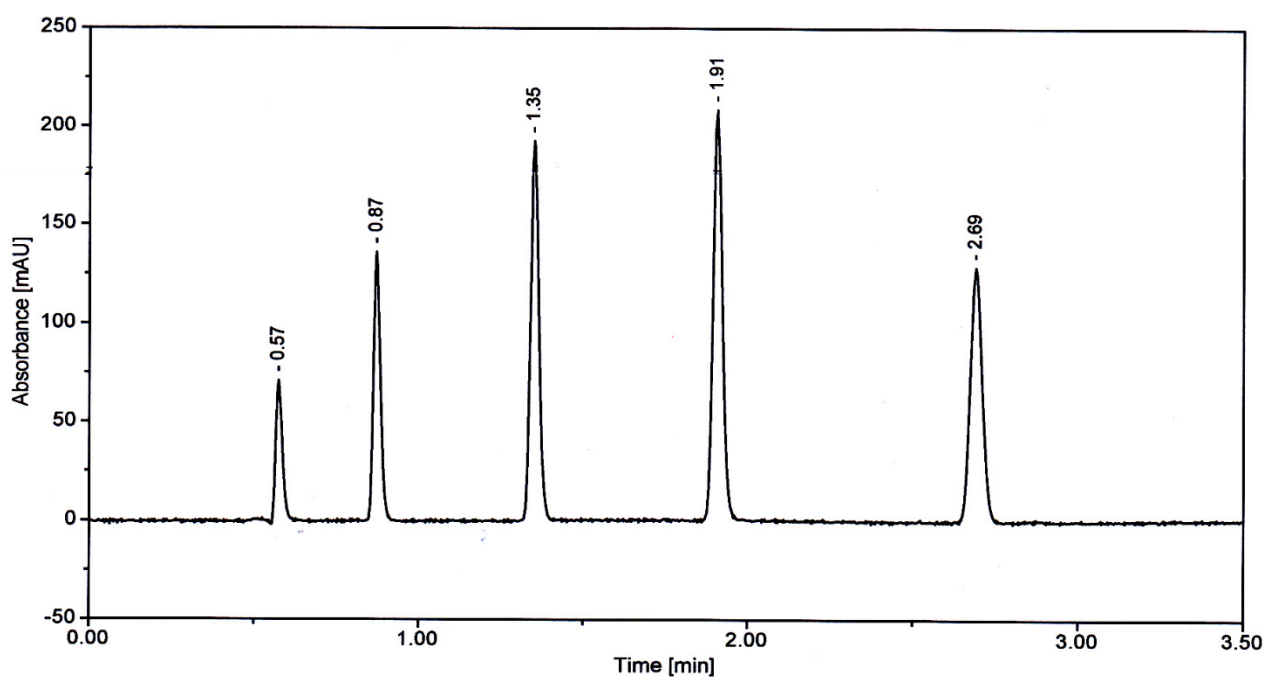
**Certificate of Analysis****LudgerSep™ UR2 UHPLC Column for Glycan Analysis**

Cat. #: LS-UR2-2.1x100

Batch: B9CC-09

Size: 2.1 x 100 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent** 50 % acetonitrile (aq)**Test Analysis****Flow Rate** 500ul / min**Eluent** Isocratic 50 % acetonitrile (aq)**Pressure** 6162 psi**Sample Volume** 1 µl**Detection** UV at 254nm

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	0.57	1.34
2	p-Nitroaniline	0.87	1.25
3	Methyl Benzoate	1.35	1.17
4	Phenetole	1.91	1.13
5	o-Xylene	2.69	1.12

Efficiency o-Xylene (n/m) = 265960

Tailing Factor (5%) o-Xylene = 1.12