



## Certificate of Analysis

---

### LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x50

Batch #: B4CN-09

Size: 2.1 x 50 mm

---

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent** 50 % acetonitrile (aq)

#### Test Analysis

**Flow Rate** 500ul / min


**Eluent** Isocratic 50 % acetonitrile (aq)

**Pressure** 4131 psi

**Temperature** Ambient

**Sample Volume** 1  $\mu$ l

**Detection** UV at 254nm

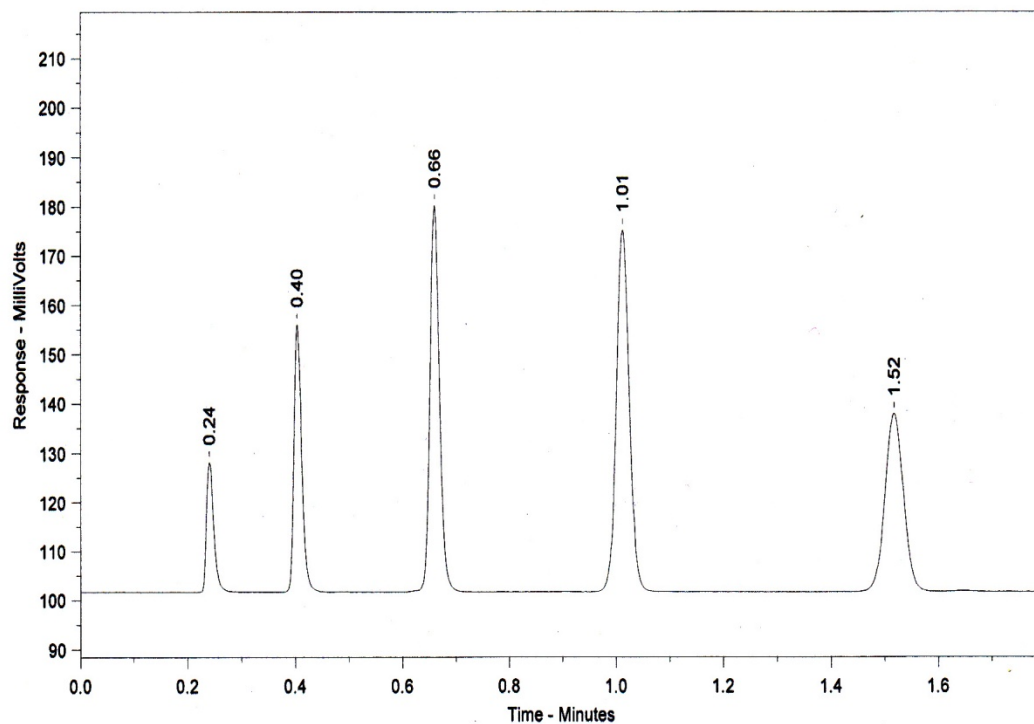

| Peak No | Peak Name       | Retention<br>time<br>(minutes) | Tailing Factor<br>(5%) |
|---------|-----------------|--------------------------------|------------------------|
| 1       | Theophylline    | 0.24                           | 1.56                   |
| 2       | p-Nitroaniline  | 0.40                           | 1.33                   |
| 3       | Methyl Benzoate | 0.66                           | 1.13                   |
| 4       | Phenetole       | 1.01                           | 1.05                   |
| 5       | o-Xylene        | 1.52                           | 1.04                   |

Efficiency o-Xylene (n/m) = 181682

Tailing Factor (5%) o-Xylene = 1.04