



Certificate of Analysis

LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x50

Batch #: B73G-07

Size: 2.1 x 50 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

Packed Solvent 50 % acetonitrile (aq)

Test Analysis

Flow Rate 500ul / min


Eluent Isocratic 50 % acetonitrile (aq)

Pressure 4017 psi

Temperature Ambient

Sample Volume 1 μ l

Detection UV at 254nm

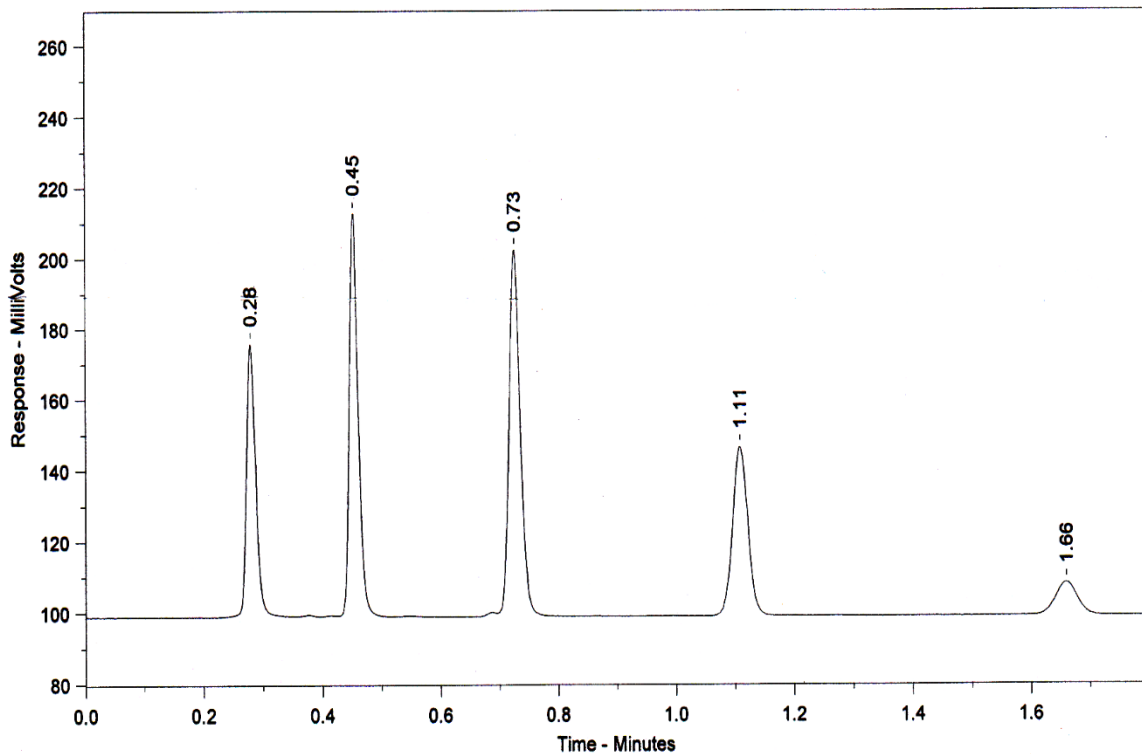

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	0.28	1.27
2	p-Nitroaniline	0.45	1.18
3	Methyl Benzoate	0.73	1.13
4	Phenetole	1.11	1.07
5	o-Xylene	1.66	1.03

Efficiency o-Xylene (n/m) = 188935

Tailing Factor (5%) o-Xylene = 1.03