



## Certificate of Analysis

---

### LudgerSep UR2 HPLC Column for Glycan Analysis

Cat. #: LS-UR2-2.1x50

Batch #: B7AU-08

Size: 2.1 x 50 mm

---

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

**Packed Solvent**      50 % acetonitrile (aq)

#### Test Analysis

**Flow Rate**            500ul / min


**Eluent**                Isocratic 50 % acetonitrile (aq)

**Pressure**             1592 psi

**Temperature**        Ambient

**Sample Volume**     1  $\mu$ l

**Detection**            UV at 254nm

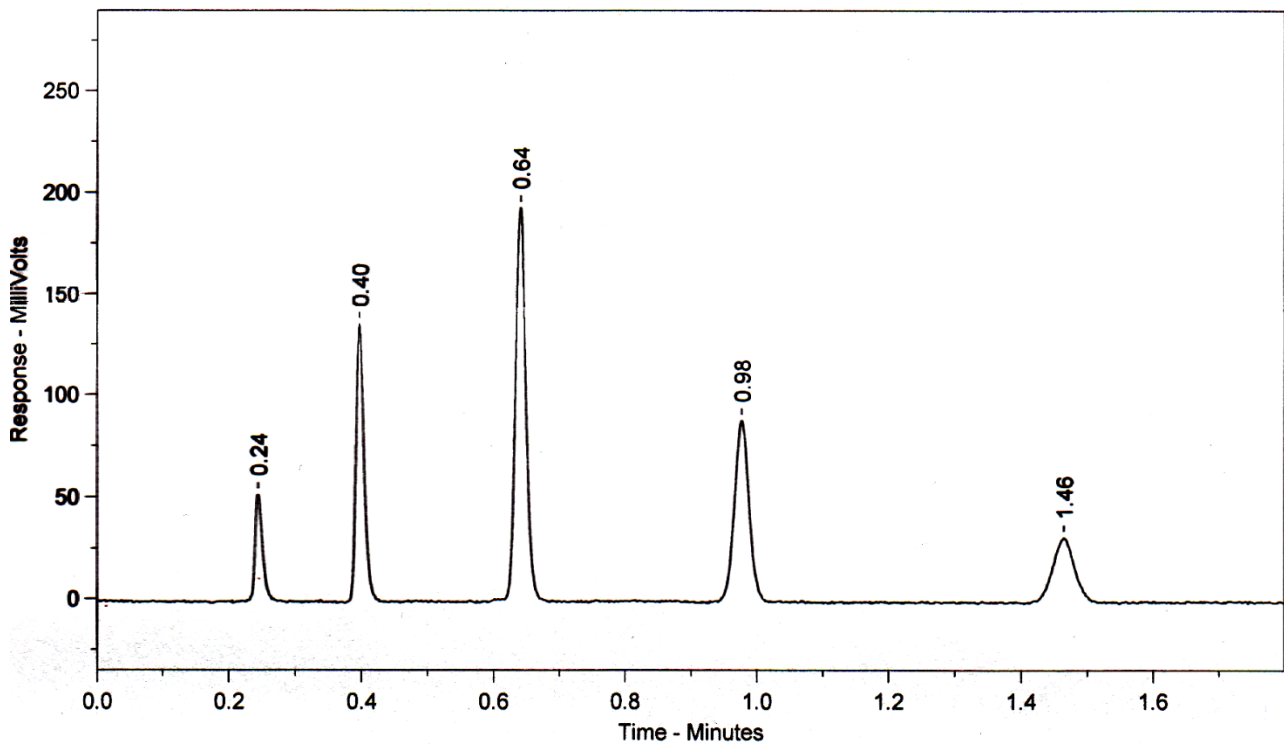

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophyline	0.24	1.36
2	p-Nitroaniline	0.40	1.36
3	Methyl Benzoate	0.64	1.18
4	Phenetole	0.98	1.04
5	o-Xylene	1.46	1.05

Efficiency o-Xylene (n/m) = 189046

Tailing Factor (5%) o-Xylene = 1.05