

Certificate of Analysis**LudgerSep™ UR2 UHPLC Column for Glycan Analysis**

Cat. #: LS-UR2-2.1x50

Batch: B8AG-02

Size: 2.1 x 50 mm

This column conforms to the specifications given in Ludger document # LS-UR2-GUIDE.

Packed Solvent 50 % acetonitrile (aq)

Test Analysis

Flow Rate 500ul / min


Eluent Isocratic 50 % acetonitrile (aq)

Pressure 3727 psi

Temperature Ambient

Sample Volume 1 µl

Detection UV at 254nm

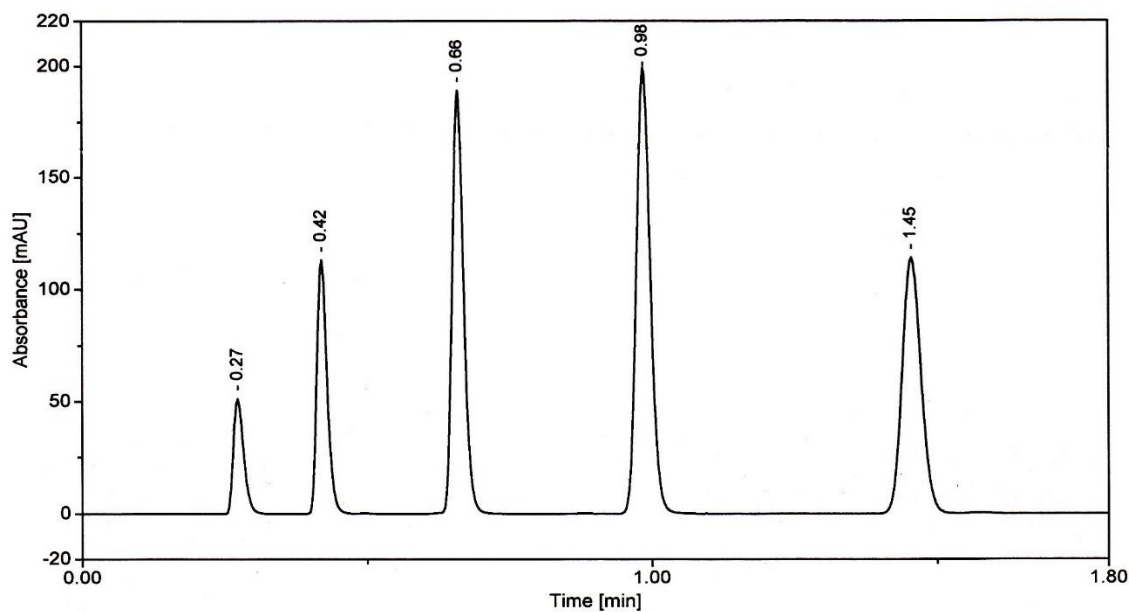

Peak No	Peak Name	Retention time (minutes)	Tailing Factor (5%)
1	Theophylline	0.27	1.34
2	p-Nitroaniline	0.42	1.28
3	Methyl Benzoate	0.66	1.20
4	Phenetole	0.98	1.12
5	o-Xylene	1.45	1.08

Efficiency o-Xylene (n/m) = 185360

Tailing Factor (5%) o-Xylene = 1.08