

Certificate of Analysis

LudgerTag™ 2-AB (2-aminobenzamide) Glycan Labeling Kit containing 2-picoline borane

Cat. #: LT-KAB-VP96

Batch: B49M-02

Size: 1 set of labeling reagents per kit

Expiry Date: 28 Nov 2019

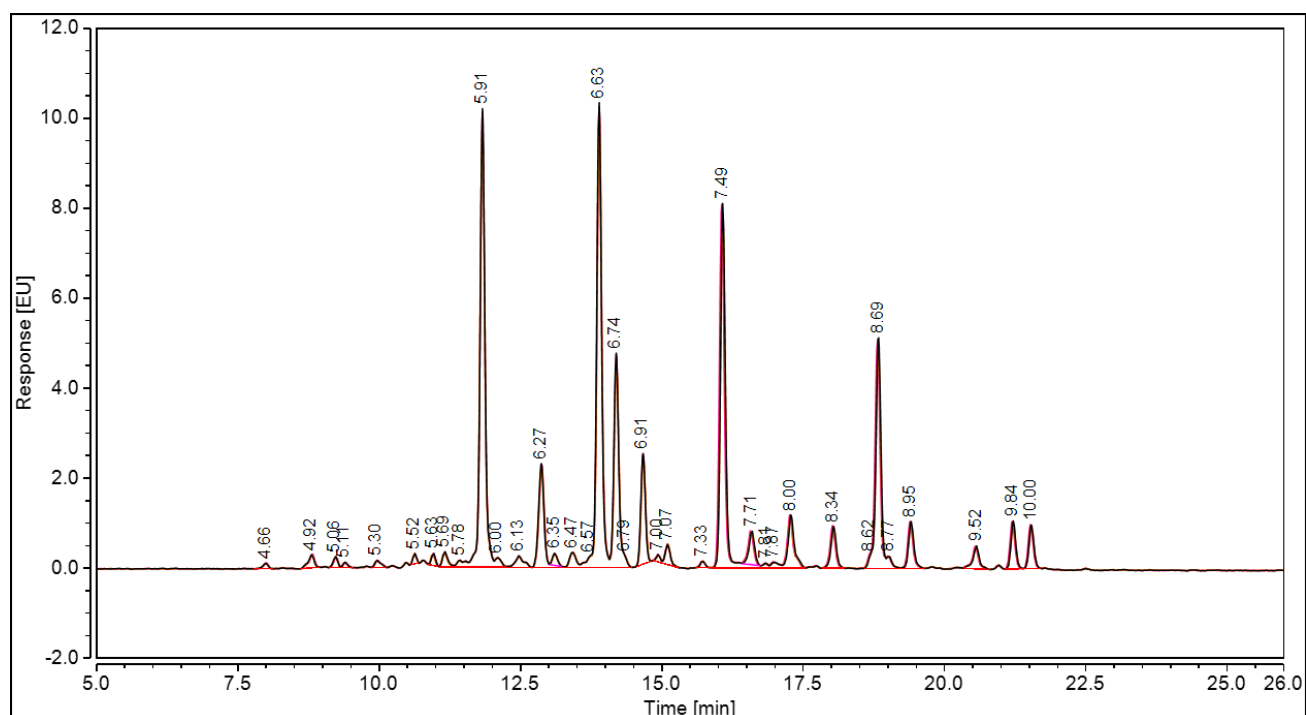


Figure 1: HILIC HPLC profile of three Human-IgG glycan samples (Cat. #: CLIBN-IGG-5U Batch B78A-01) labeled using LT-KAB-VP96 (Batch B49M-02)

HPLC Running Conditions:

Column: Waters BEH Glycan column (1.7µm-2.1x150)

Flow: 0.56 mL/min

Solvent A: 50 mM ammonium formate pH 4.4

Solvent B: 100 % acetonitrile

Temperature: 60 °C.

Gradient: 0 min – 78% B, 1.47 min – 78% B, 24.80 min – 58% B, 25.8 min – 40% B, 25.9 min – 78% B, 31.0 min – 78% B

Detector: Dionex FLD-3000

Excitation wavelength: 250 nm

Emission wavelength: 428 nm