

Certificate of Analysis

LudgerTag™ Procainamide Glycan Labeling Kit

Cat. #: LT-KPROC-96

Batch: B96A-05

Size: 1 set of labeling reagents per kit

Expiry Date: 25 Jan 2020

This kit conforms to the specifications given in Ludger document # LT-KPROC-96-Guide.

Each kit contains the following components:

Quantity per Kit	Cat #	Batch #	Component Name
1	LT-ACETIC-DMSO-96	B81U-07	Acetic Acid with DMSO
1	LT-PROC-96	B81U-06	Procainamide
1	LT-CYANOB-96	B965-10	Sodium Cyanoborohydride

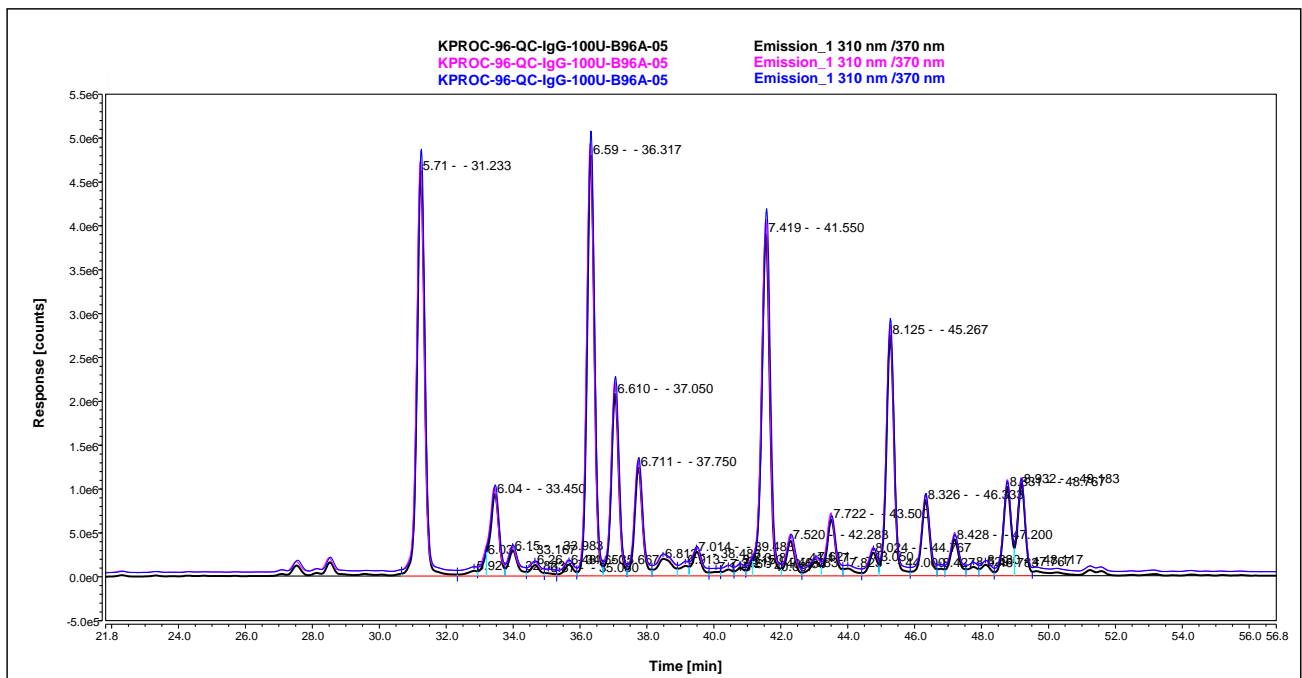


Figure 1: BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from human IgG by PNGase F digestion