

Certificate of Analysis

LudgerTag™ Procainamide Glycan Labelling Kit

Cat. #: LT-KPROC-96

Batch: B99I-04

Size: 1 set of labeling reagents per kit

Expiry Date: 07 Jun 2021

This kit conforms to the specifications given in Ludger document # LT-KPROC-96-Guide.

Each kit contains the following components:

Quantity per Kit	Cat #	Batch #	Component Name
1	LT-ACETIC-DMSO-96	B99G-01	Acetic Acid with DMSO
1	LT-PROC-96	B98T-01	Procainamide
1	LT-CYANOB-96	B965-10	Sodium Cyanoborohydride

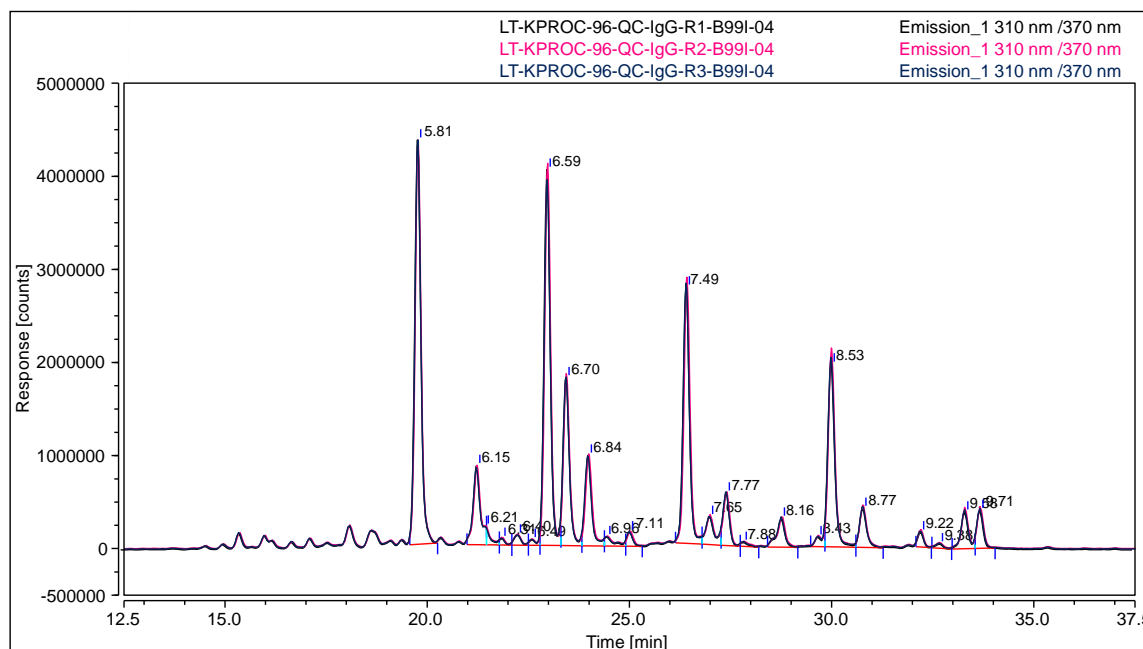


Figure 1: BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from human IgG by hydrazinolysis.