



Ludger

Certificate of Analysis

LudgerTag procainamide Glycan Labelling Kit

Cat. #: LT-KPROC-24

Batch #: B63T-02

Size: 2 sets of labeling reagents per kit

This kit conforms to the specifications given in Ludger document # LT-KPROC-24-Guide.

Each kit contains the following components:

Quantity per Kit	Cat #	Batch #	Component Name
2	LT-ACETIC-DMSO-01	B4BI-01	acetic acid with DMSO
2	LT-PROC-01	B63A-01	procainamide
2	LT-CYANOB-05	B63O-02	sodium cyanoborohydride

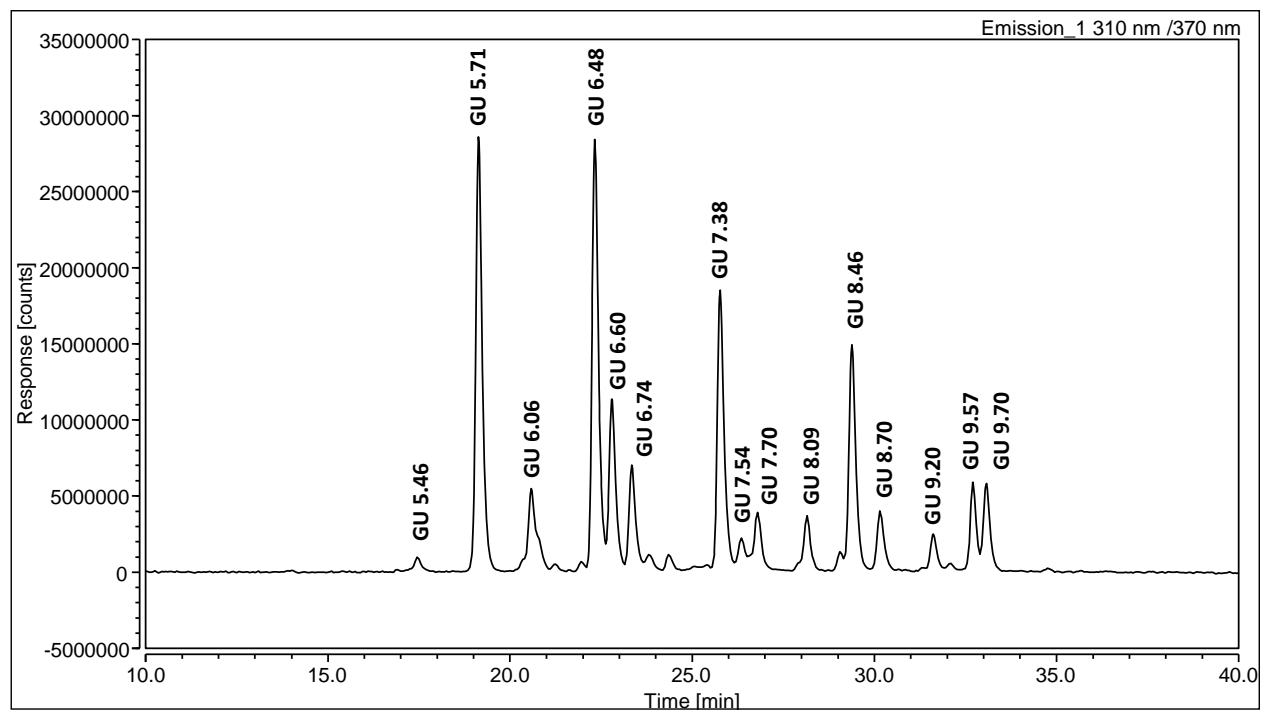


Figure 1. BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from human IgG by PNGase F digestion

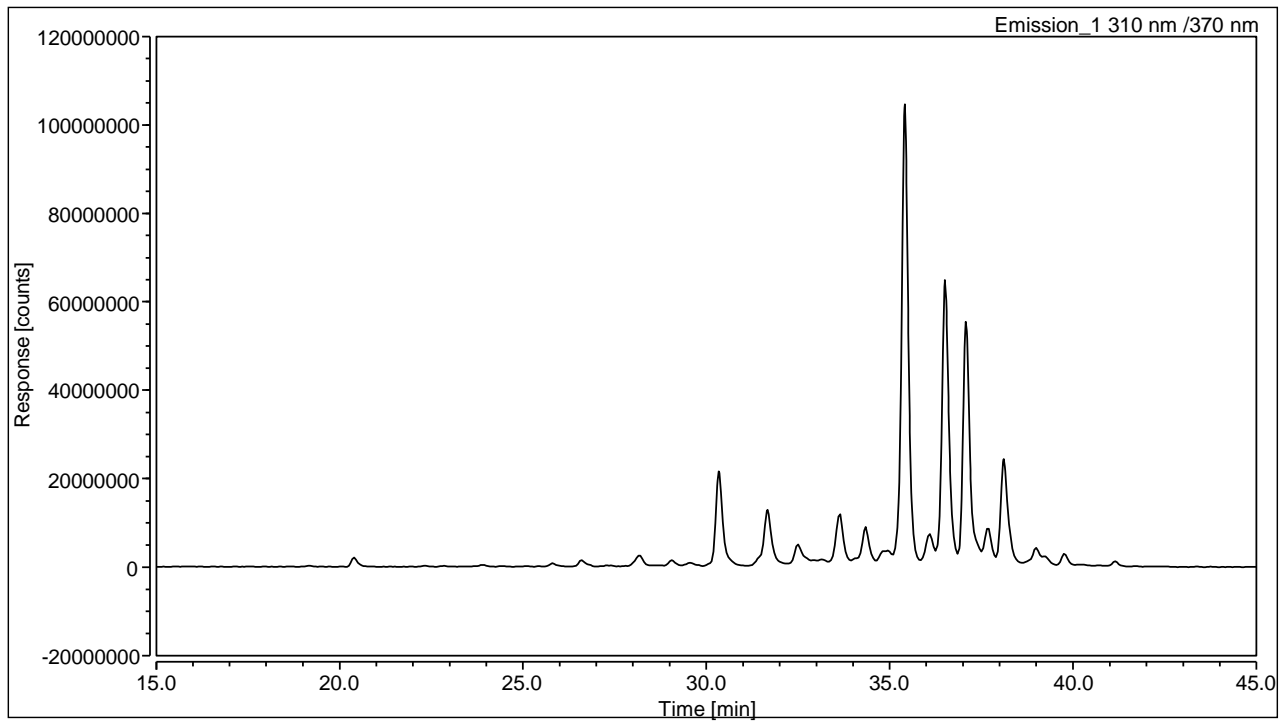


Figure 2. BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from bovine fetuin by PNGase F digestion