

## Certificate of Analysis

### LudgerTag™ Procainamide Glycan Labeling Kit

Cat. #: LT-KPROC-24

Batch: B97V-04


Size: 2 sets of labeling reagents per kit

Expiry Date: 25 May 2021

This kit conforms to the specifications given in Ludger document # LT-KPROC-24-Guide.

Each kit contains the following components:

Quantity per Kit	Cat #	Batch #	Component Name
2	LT-ACETIC-DMSO-01	B85P-01	Acetic Acid with DMSO
2	LT-PROC-01	B97U-05	Procainamide
2	LT-CYANOB-05	B865-01	Sodium Cyanoborohydride

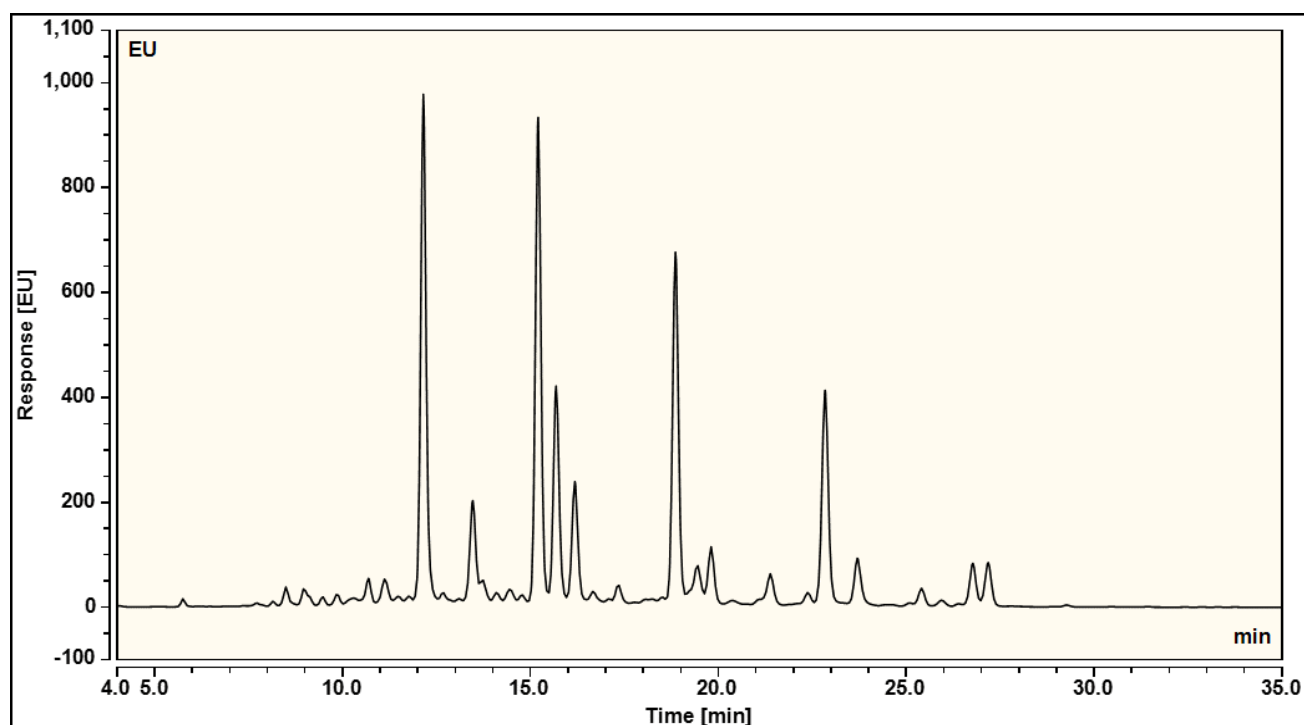

**Figure 1:** BEH Glycan column UHPLC profile of procainamide labeled N-glycans released from human IgG and labelled using LT-KPROC-24